



Biosensors

- Biosensing principles and figure of merits
- Optical biosensors
 1. DNA/protein microarrays
 2. Surface plasmon resonance (SPR)
 3. Surface-enhanced Raman scattering (SERS)
 4. Zero-mode waveguide
- Electrical biosensors
 1. Electrochemical (ECM) sensors
 2. Field-effect transistor (FET) sensors
 3. Nanopore sensors
- Mechanical biosensors
 1. Cantilever sensors



Fundamental Design and Operational Considerations for Affinity-Based Biosensors

Structural and design considerations

Bioaffinity element properties

Assay format

Sensor material

Transducer type

Operational considerations

Sensitivity, selectivity,
kinetic parameters, stability

Homogeneous vs heterogeneous
reversible, regenerable, disposable
continuous, remote, *in situ* operation
assay time

Immobilization method

Mechanism of signal transduction



Bioaffinity Elements for Affinity-Based Biosensors

Bioaffinity element	Types of analyte	Examples
Antibodies	Low mol-wt compounds Proteins Microorganisms	Drugs, hormones, environmental pollutants (pesticides, explosives, and so forth) Antipathogen antibodies Toxins, insulin, serum proteins <i>Candida albicans</i> , <i>Escherichia coli</i> , <i>Salmonella typhimurium</i> , <i>Salmonella dysenteria</i> , <i>Yersinia pestis</i>
Biological receptors -Interleukin-6 receptor -Acetylcholine receptor	Physiological ligands Pharmacological ligands Toxicological ligands	Nicotine, carbamyl choline Bungarotoxin
Nucleic acids	Identification of specific sequences, Detection of intercalators	<i>Legionella pneumophila</i> Ethidium, PAHs



Signal Transducers for Affinity-Based Biosensors

Transducer type	Assay format
Optical	
Fluorescence energy transfer	Direct
Bioluminescence	Indirect
TIRF ^a	Direct
SPR ^b	Direct
Grating coupler	Direct
Electrochemical	
Potentiometric	Indirect, direct
Amperometric	Indirect
Conductimetric	Indirect
Thermal	Indirect
Acoustic	Direct
QCM ^c	

^aTotal internal reflectance fluorescence

^bSurface plasmon resonance

^cQuartz crystal microbalance



Basic components of an affinity-based biosensor?

- Analyte
- Biorecognition (sensing) element
- Transducer (reporting element)




Types of Applications

- Medical diagnostics (pathogens, diseases)
- Drug target discovery
- Forensics
- Food and environmental
- Genomic/Proteomic research
 - DNA analysis
 - mRNA analysis
 - Protein analysis
 - Disease-Gene association
 - Pharmacogenomics /pharmacogenetics




Monitor molecular interactions


Protein interactions

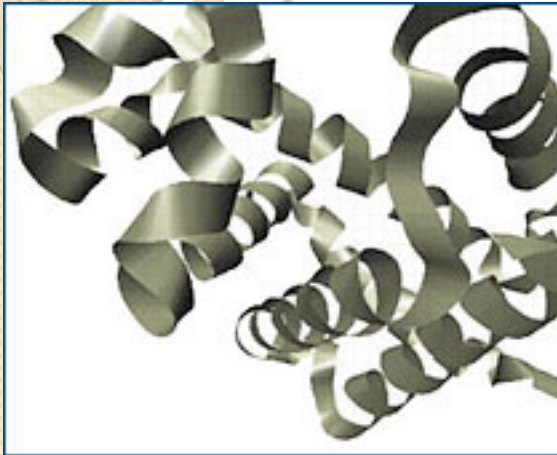

Small molecules

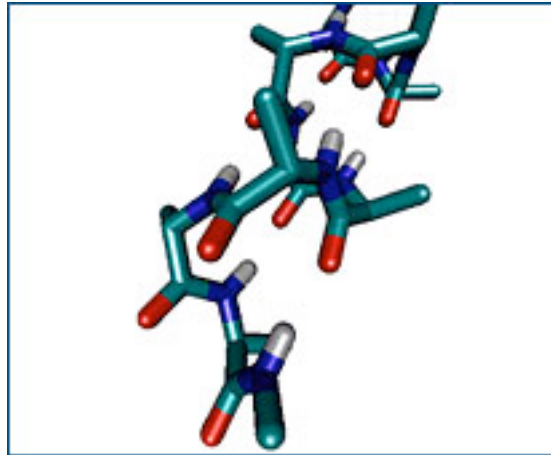

Membrane proteins

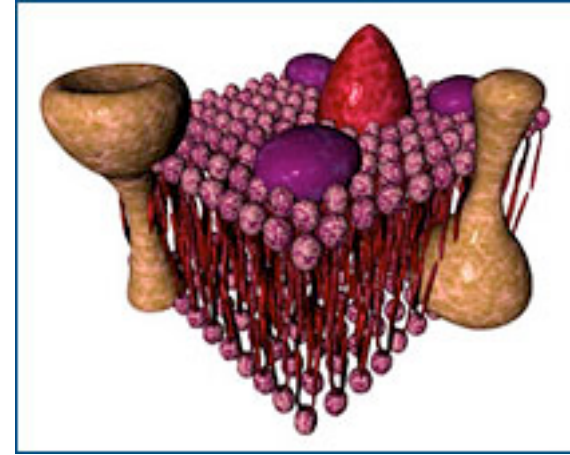

Nucleic acids



Cell and viruses




Carbohydrates






Direct assay format of biosensors

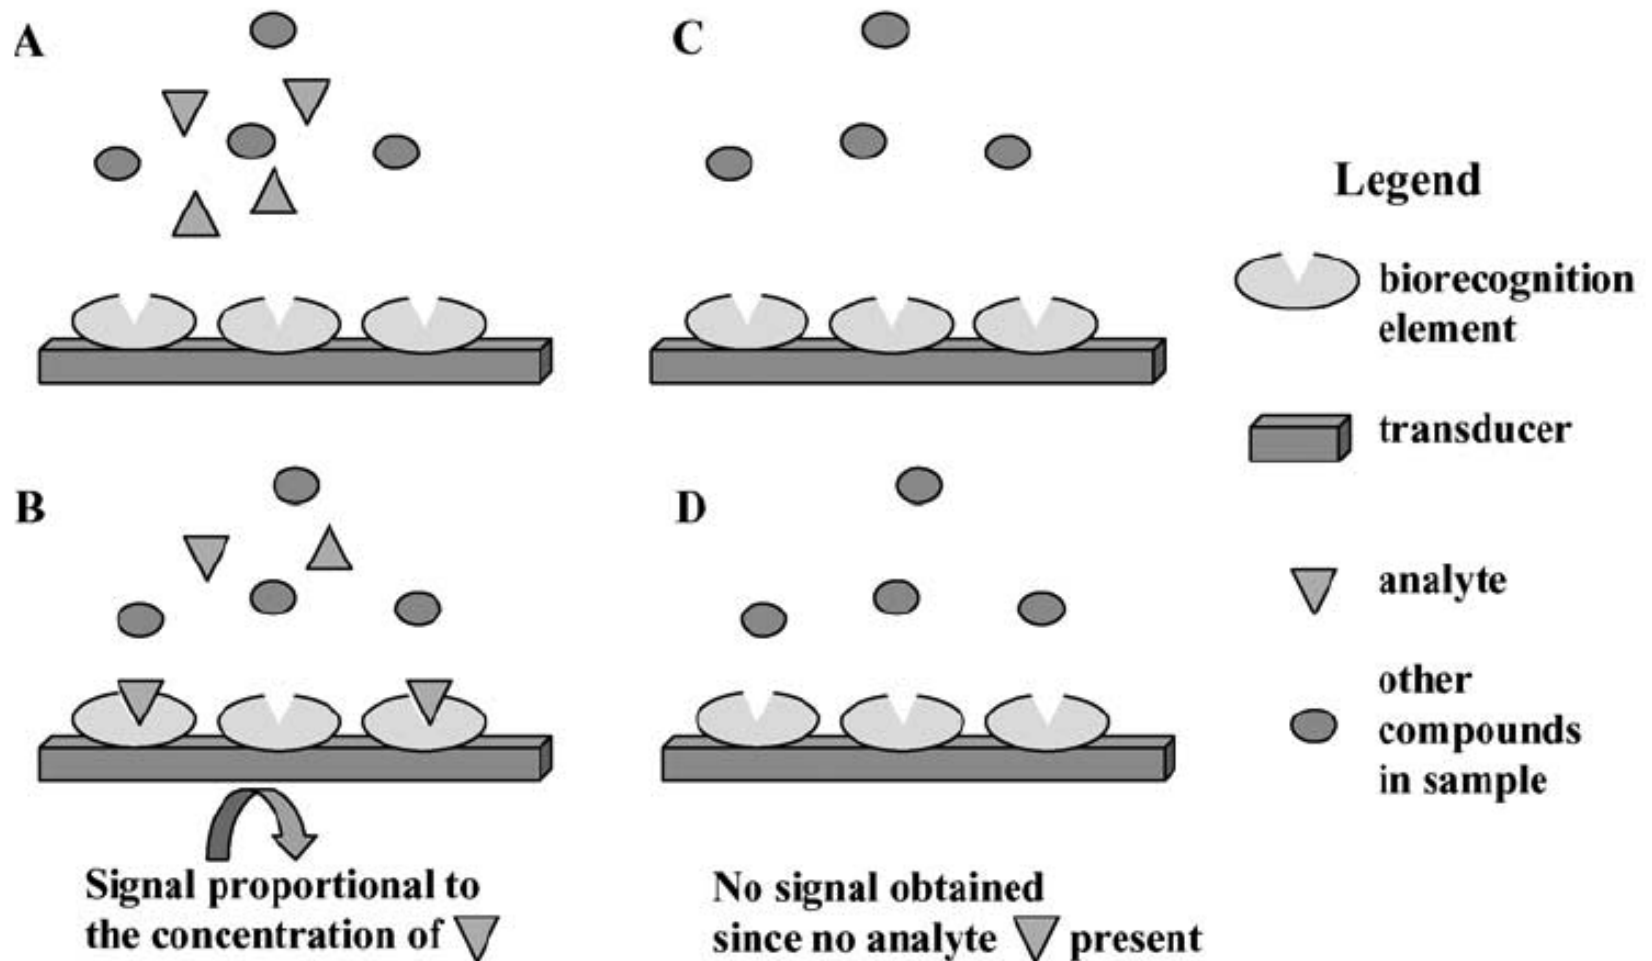




Indirect assay format with competitive binding

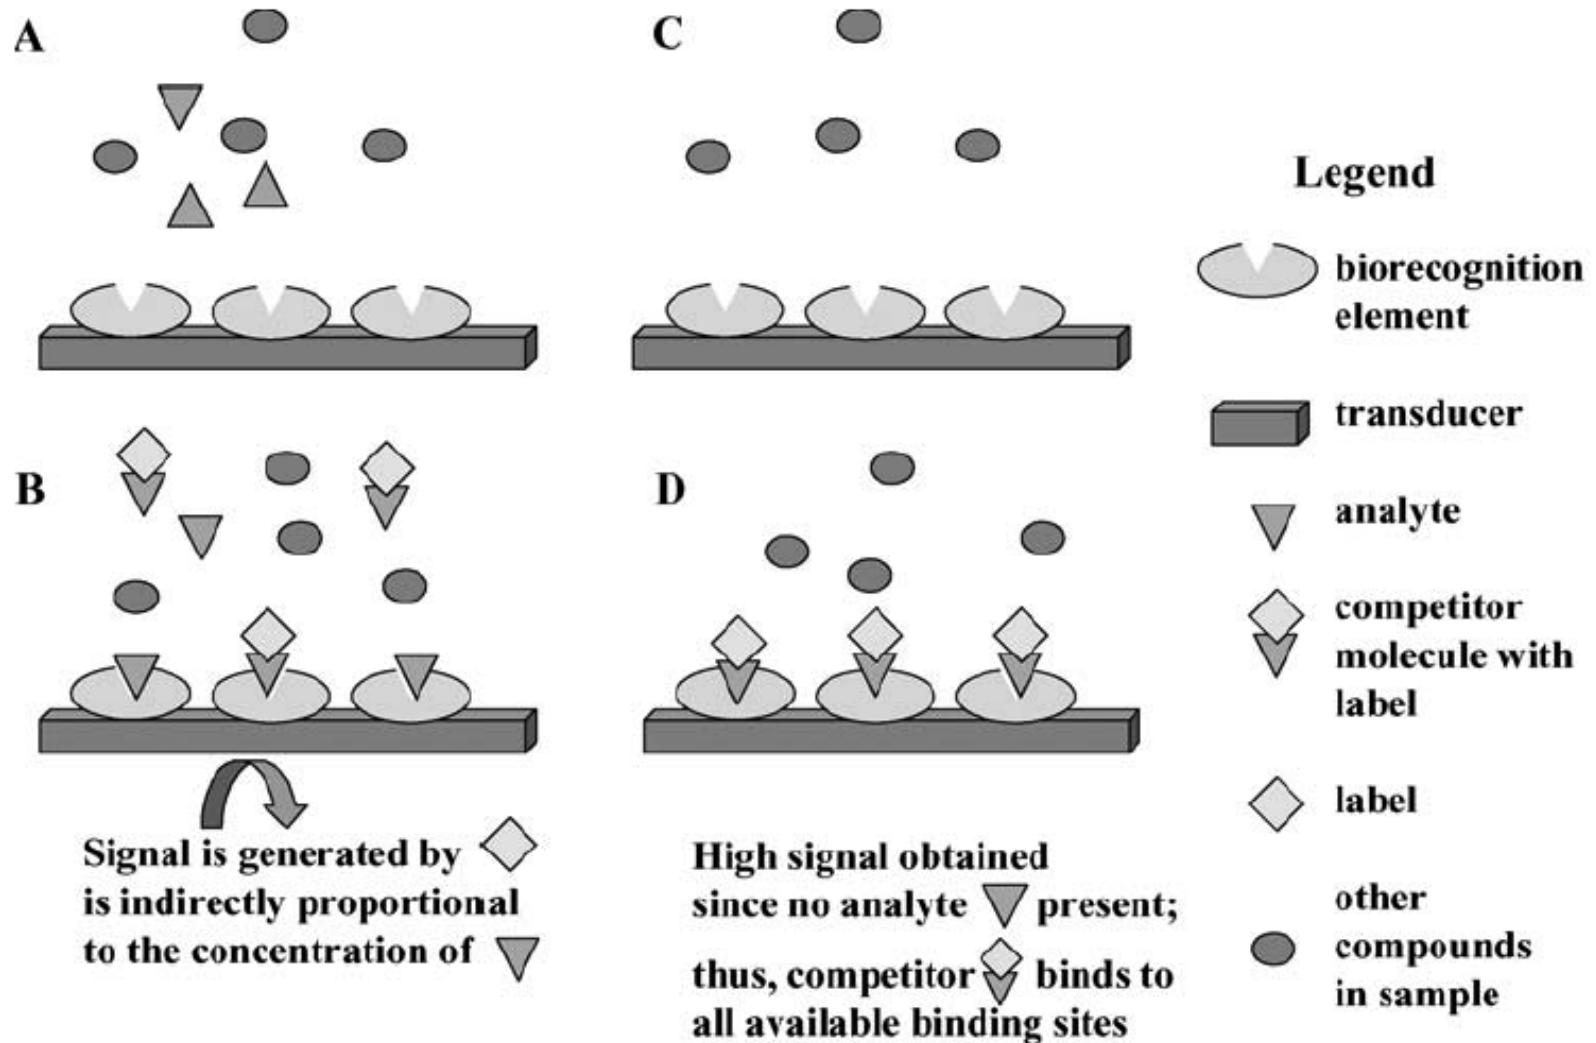




Indirect assay format with non-competitive binding

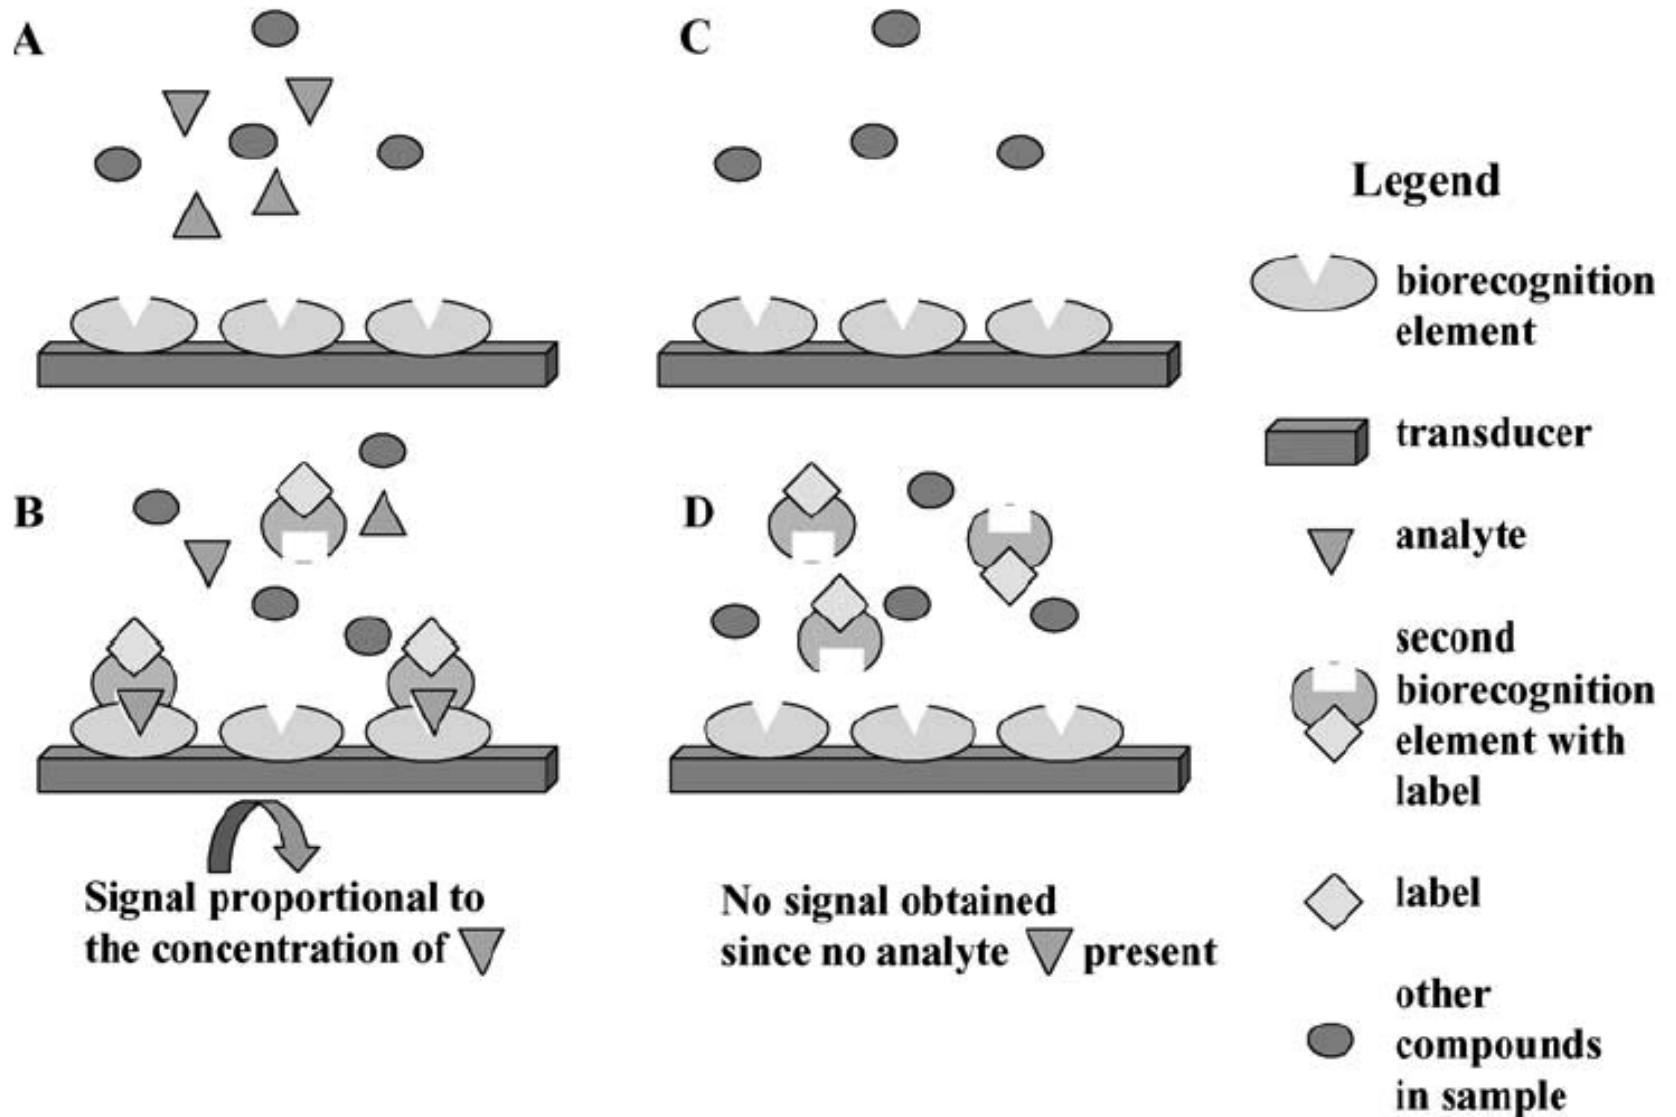



Enzyme-linked immunosorbent assay (ELISA)

a biochemical technique used mainly in immunology to detect the presence of an antibody or an antigen in a sample.

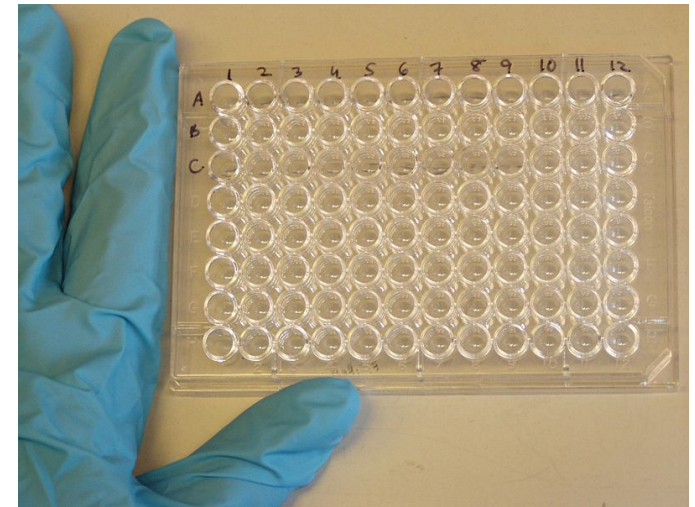

A 96-well microtiter plate being used for ELISA

(1)


(2)

(3)

(4)

(5)

Sandwich ELISA

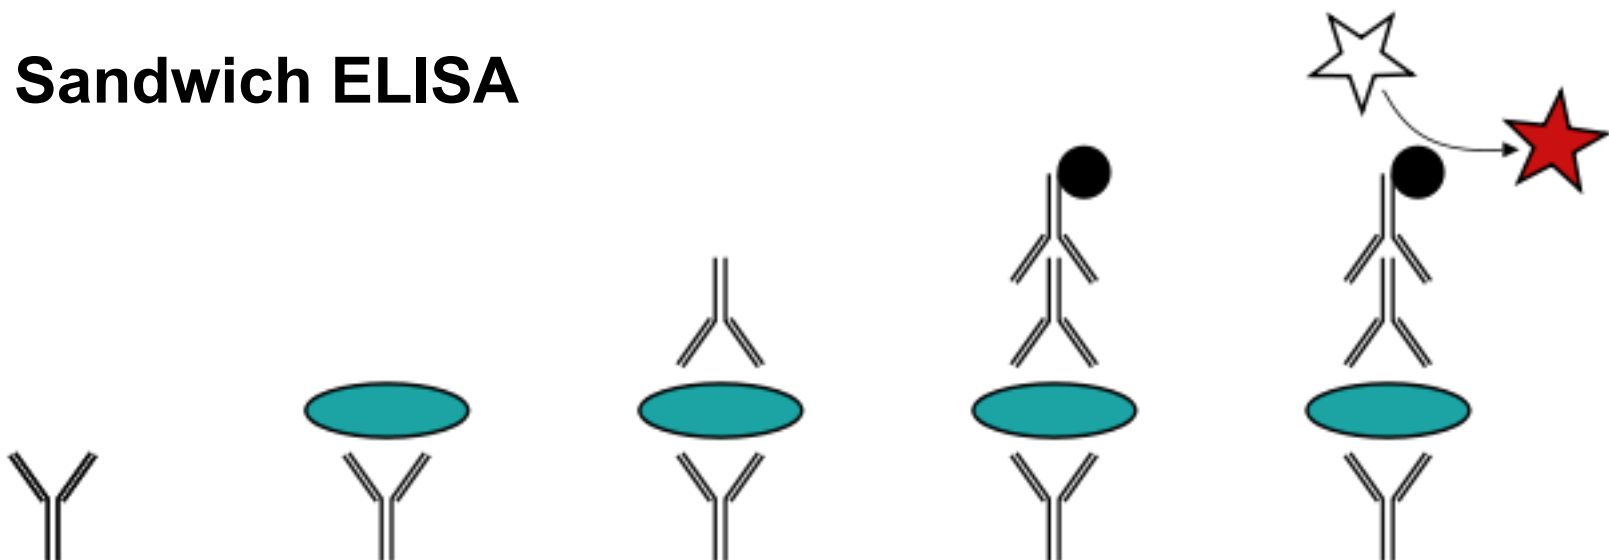

A cytokine ELISA assay

A Cytokine ELISA Assay

- 1) Coat microwell with anti-cytokine capture antibody



Animation provided by:


CTL

Cellular Technology Ltd.

www.immunospot.com
www.elispot-analyzers.de
www.elispot.cn
www.elispot.co.jp



Principles of DNA Hybridization & Sensing

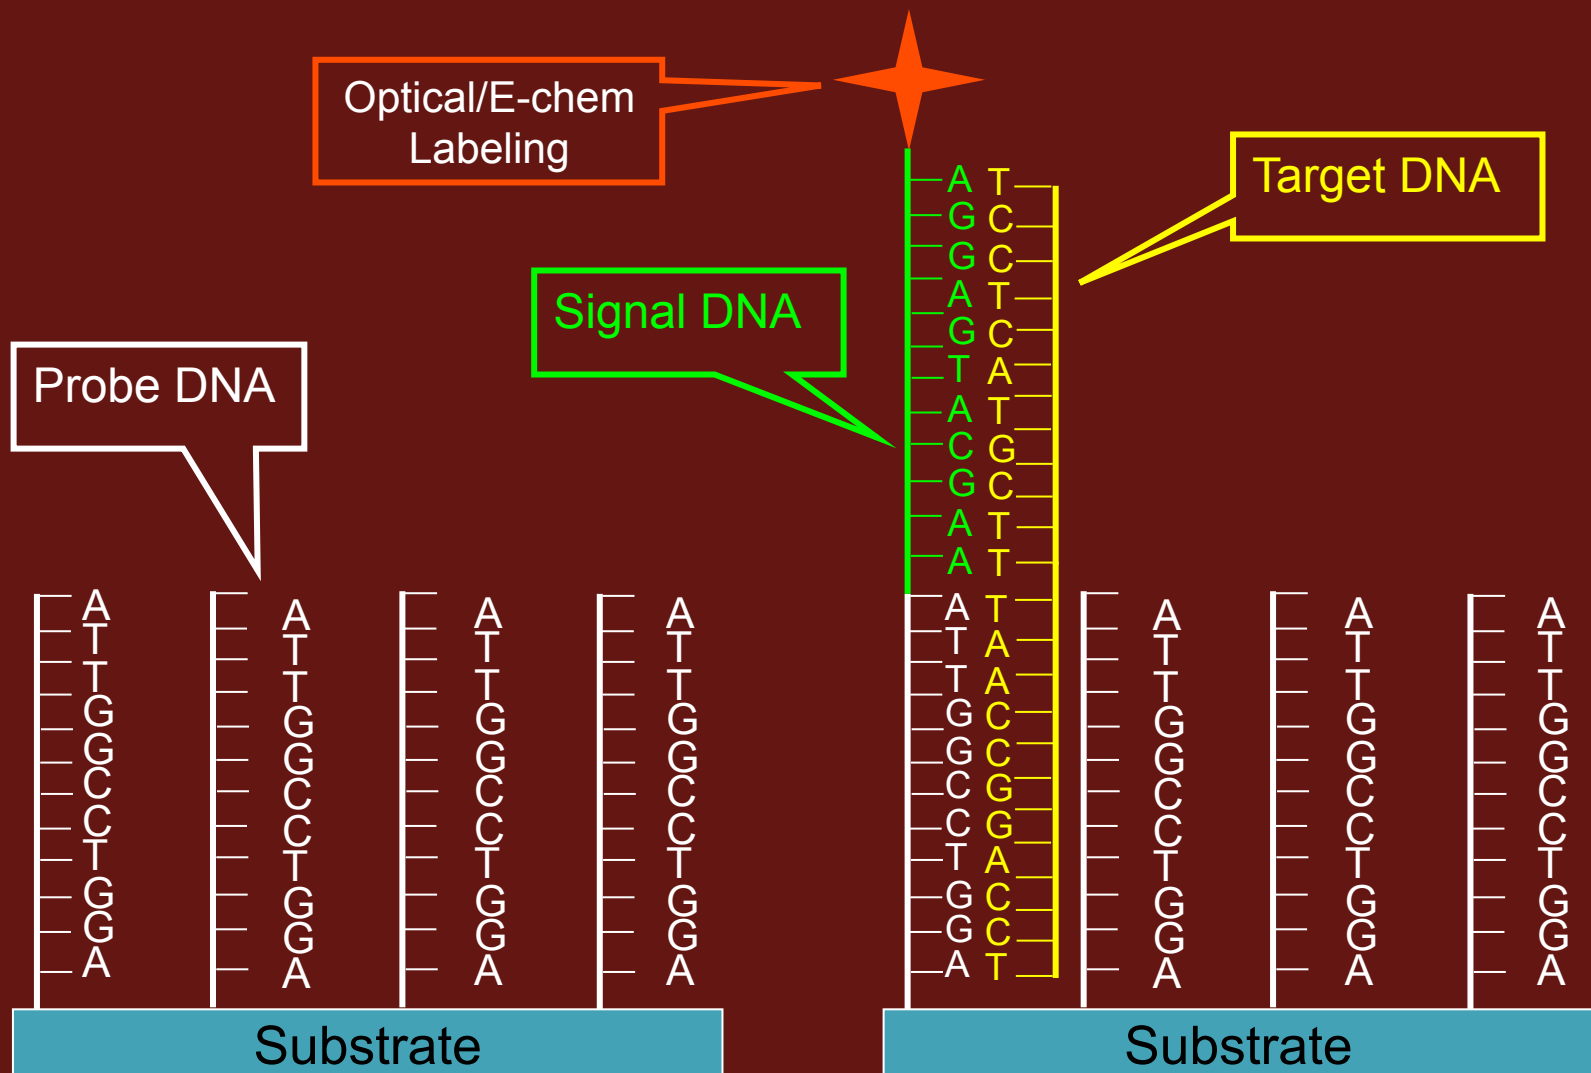



Different DNA hybridization array formats

	Probe generations method	Array size	Labeling and detection method	Hybridization method	Commercial suppliers
Microarrays [5]	Robotic printing or piezoelectric inkjet printing of PCR products	2.5 cm by 7.5 cm slide with approximately 10 000 genes	Fluorescent tag labeling prior to hybridization; fluorophore added after hybridization and washing	Passive	Agilent Technologies, Genometrix, Operon Technologies, Stratagene
Oligonucleotide arrays [6]	<i>In-situ</i> on the surface of the matrix	1 cm by 1 cm slide with approximately 40 000 genes; Affymetrix's GeneChip can contain up to 400 000 different oligonucleotides and is the densest array	Fluorescent tag labeling; fluorophore detector is added after hybridization	Passive	Affymetrix
Macroarrays [7]	Probes are spotted onto nylon, plastic or nitrocellulose solid matrix	8 cm by 12 cm with approximately 200 to 5000 genes	Radioactivity tag labeling; phosphorimager detector	Passive	Clontech Laboratories, Research Genetics
Microelectronics arrays [8]	Probes are drawn by electric current to chip surface	Number of genes is dependent on the number of electrodes that can be made onto the surface of the array	Fluorescent tag labeling and fluorescent detection	Active	Nanogen



Different array generation approaches

	Spatial resolution	Cost	Probe length	Ease of use
Robotic microprinting	Poorest	Most cost effective	Not restricted	Requires cloning and PCR steps
Photolithography	Highest	Highest as expensive equipments and particular expertise are required	Limited to 25-mers or less	Photolithography method is protected by patent and currently only Affymetrix has the rights to use this method
Inkjet printing	In between robotic printing and photolithography	In between robotic printing and photolithography	5–75-mers	Equipments need strict maintenance and experiment must be performed in a clean and uncontaminated environment

The first GeneChip (late 1980's)



Revolutionary idea:


Semiconductor manufacturing techniques could be united with advances in combinatorial chemistry to build vast amounts of biological data on a small glass chip.

By Stephen P.A. Fodor, Ph.D., Affymetrix Founder,
Chairman and CEO


Source: www.affymetrix.com

The first GeneChip (late 1980's)

Photolithographic synthesis of oligonucleotide probe arrays

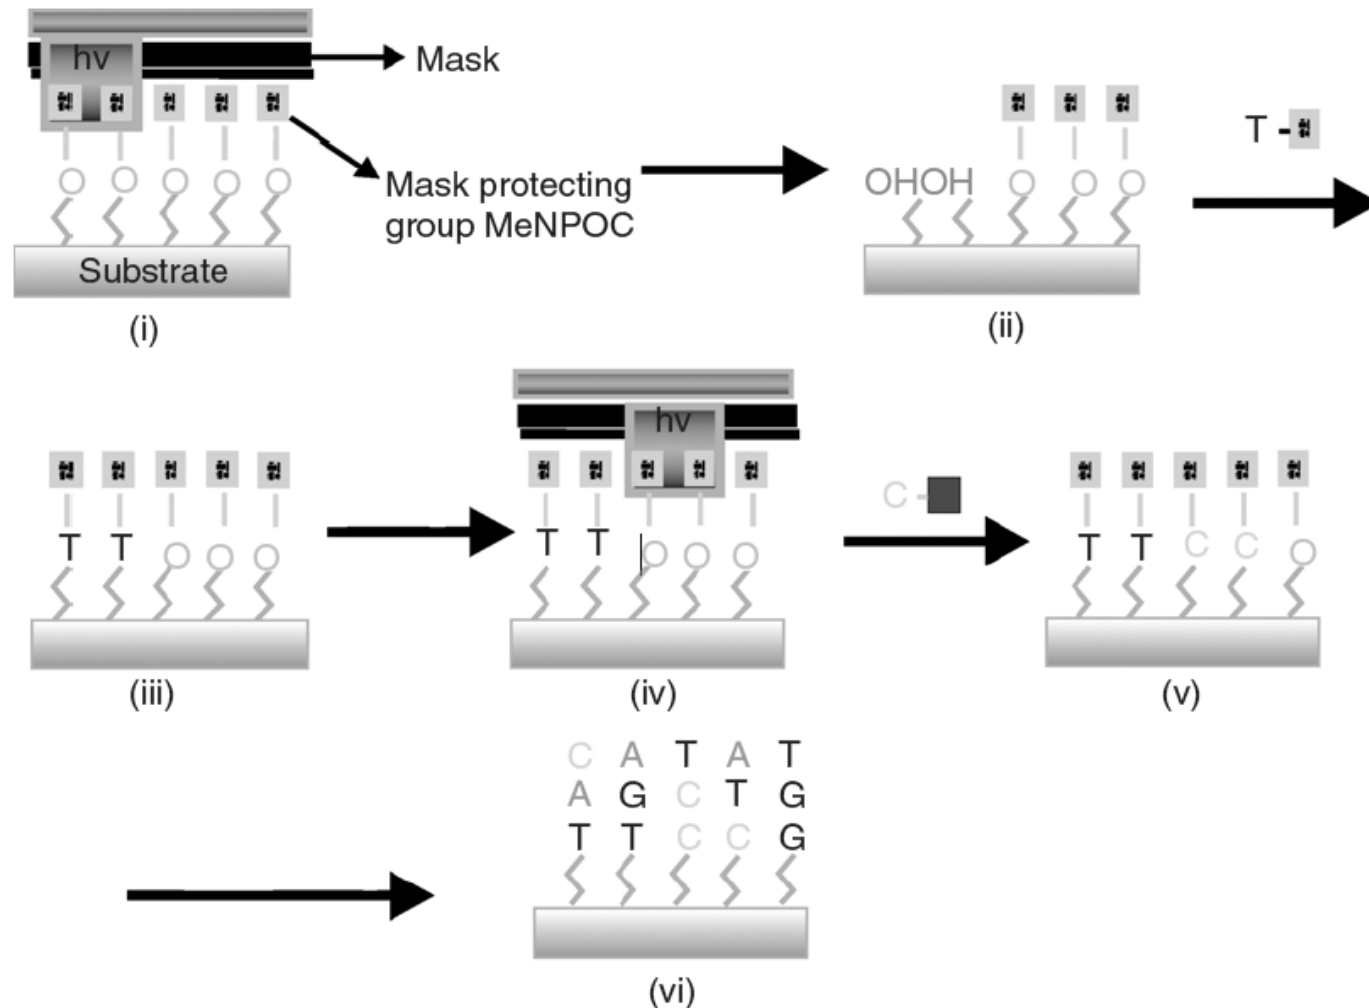

Affymatrix GeneChip

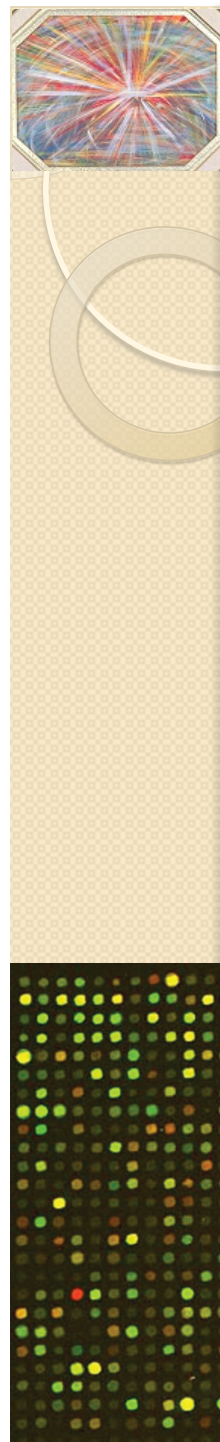

GeneChip® Probe Array

1.28 cm

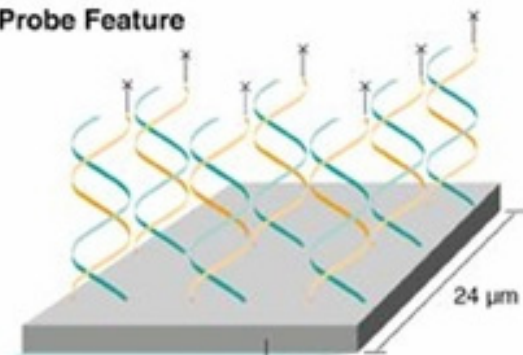


Image of Hybridized Probe Array

Hybridized Probe Feature

Single stranded, fluorescently labeled DNA target


Oligonucleotide probe



24 μm

Each probe feature contains millions of copies of a specific oligonucleotide probe

Over 200,000 different probes complementary to genetic information of interest

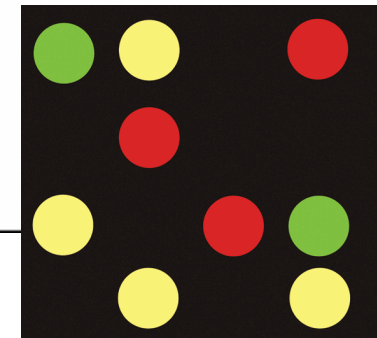


Ideal microarray spots

Source: www.affymetrix.com




Printhead with a series of pins (robotic microprinting)

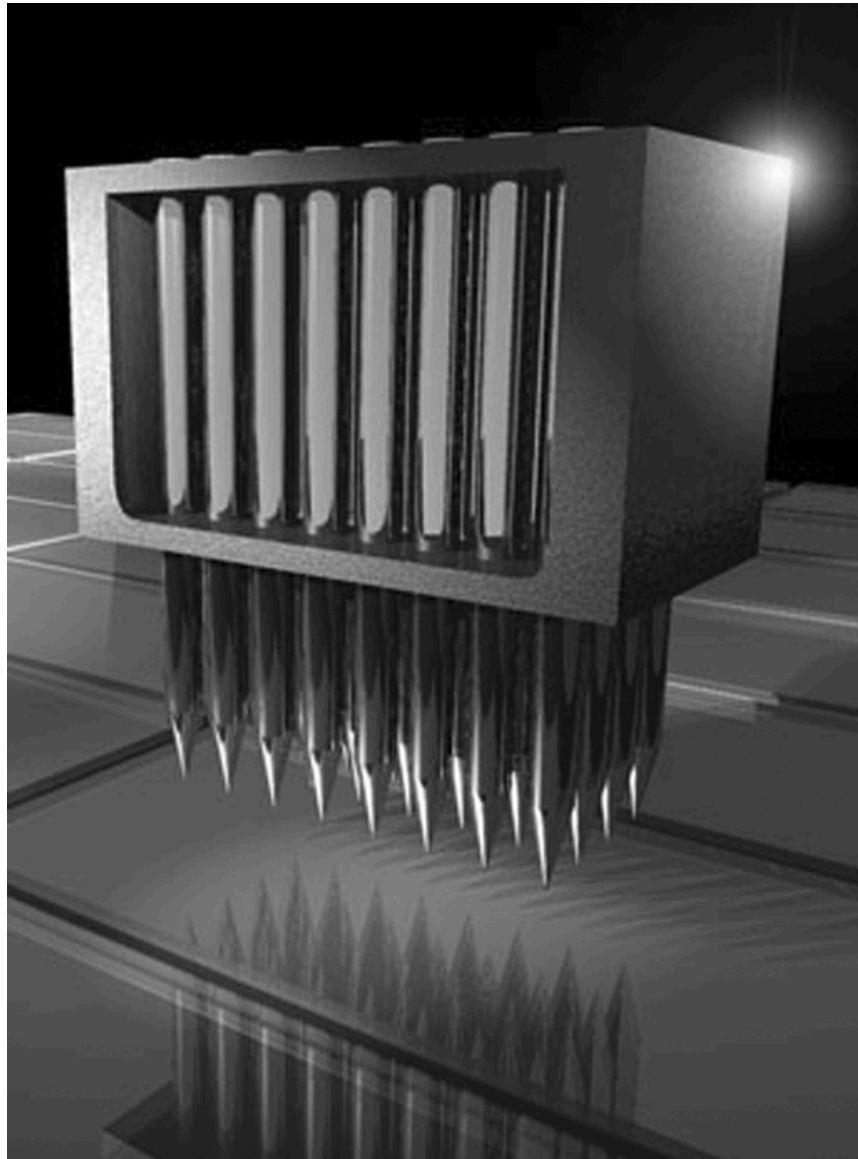

Source: <http://cmgm.stanford.edu/pbrown/>



Biochip Fabrication by inkjet/piezoelectric methods

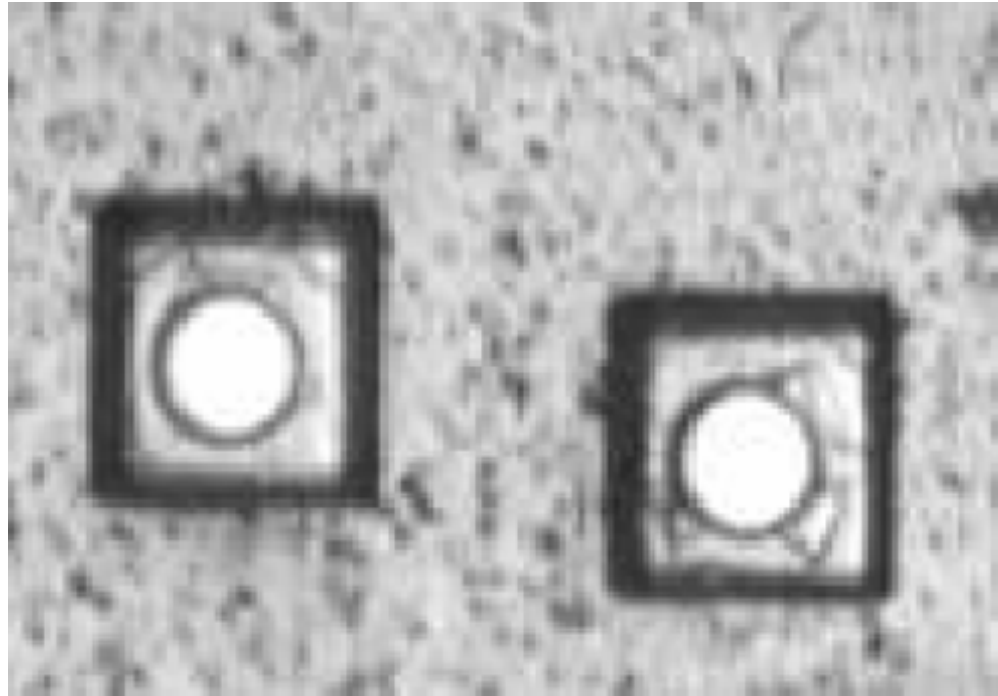

Orifice plate with 40 μm diameter orifices

Data from inkjet printing method

Dispense volume	Spot sizes	Spot densities	Delivery speed
50 pL	125–175 μm	500–2500 spots/ cm^2	100–500 spots/s



Detection limits of various techniques for DNA hybridization

Detection method	Detection limit (concentration of target molecules)	Sample volume	Detection limit (no. of hybridized target molecules)	Refs
Flourescence	5 pM	10–50 μ l	10^3 per 100 x 100 μ m spot	Taton et al., 2000; Duggan et al., 1999
“Scanometric” (nanoparticle-based)	50 fM			Taton et al., 2000
Surface plasmon resonance (label-free)	10 nM		6×10^8 per 500 x 500 μ m spot	Nelson et al., 2001
Surface plasmon resonance (Au-amplified)	10 pM			He et al., 2000
Dye-containing liposomes	220 pM		6×10^8	Rule et al., 1996
BARC sensor (magnetic beads)	100 fM (using optical detection)			Edelstein et al., 2000
Microcantilever deflection	400 nM		10^{10}	Fritz et al., 2000
Molecular beacons	100 pM	10 μ l		Steemers et al., 2000
electrochemical	100pM-100 fM	500 μ l	10^8 per 100 μ m pad	Umek et al., 2001 Motorola Life sciences data
Optical interference	10 fM	10–25 μ l		Jenison et al., 2001




Nano Optical Biosensors

- ❖ Manipulation and confining of light at sub-wavelength length scale by engineering surface plasmons
- ❖ Biomolecular signal amplifications
- ❖ Unique opportunities for interfacing with biomolecules especially proteins and drug molecules at extremely small spatial scales, for practical applications such as biosensing, single molecule kinetics, and drug safety and efficacy studies

- a. NanoPair – DNA sensor
- b. NanoBurger— Engineered Hotspots for Protein SERS
- c. Nanopore sensors


Surface Plasmon Resonance (SPR)

Enhanced local-field

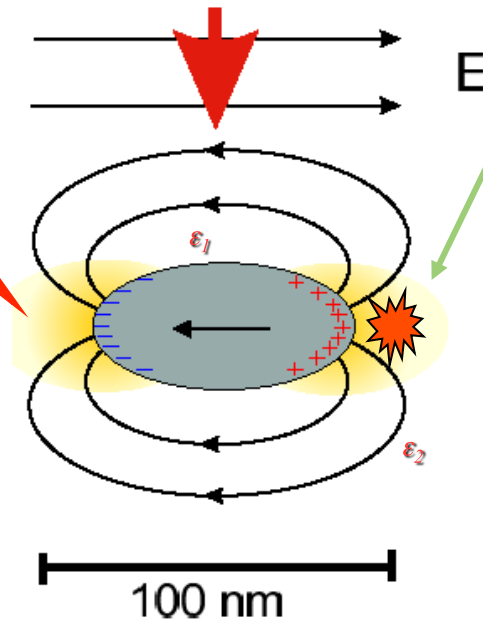

$$P \sim \frac{\epsilon_1 - \epsilon_2}{\epsilon_2 - d[\epsilon_1 - \epsilon_2]}$$

Enhanced Raman Signals (SERS)

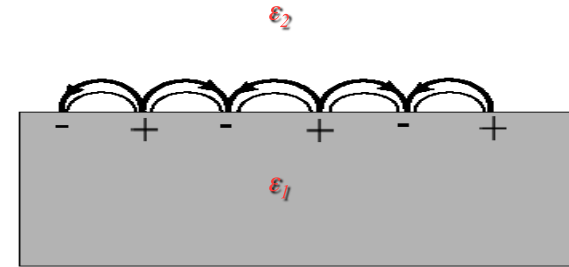

$$k = \frac{\omega}{c} \sqrt{\frac{\epsilon_1 \epsilon_2}{\epsilon_1 + \epsilon_2}}$$


Advantages of SERS:

1. Direct molecular fingerprints
2. Multiplexed detection
3. Single-molecule sensitivity
4. No photobleaching


State-of-the-art of SERS substrates:

1. Colloid particles, not compatible with microfabrication processes
2. Unrepeatable enhancement factor

SPR-Kretschmann configuration

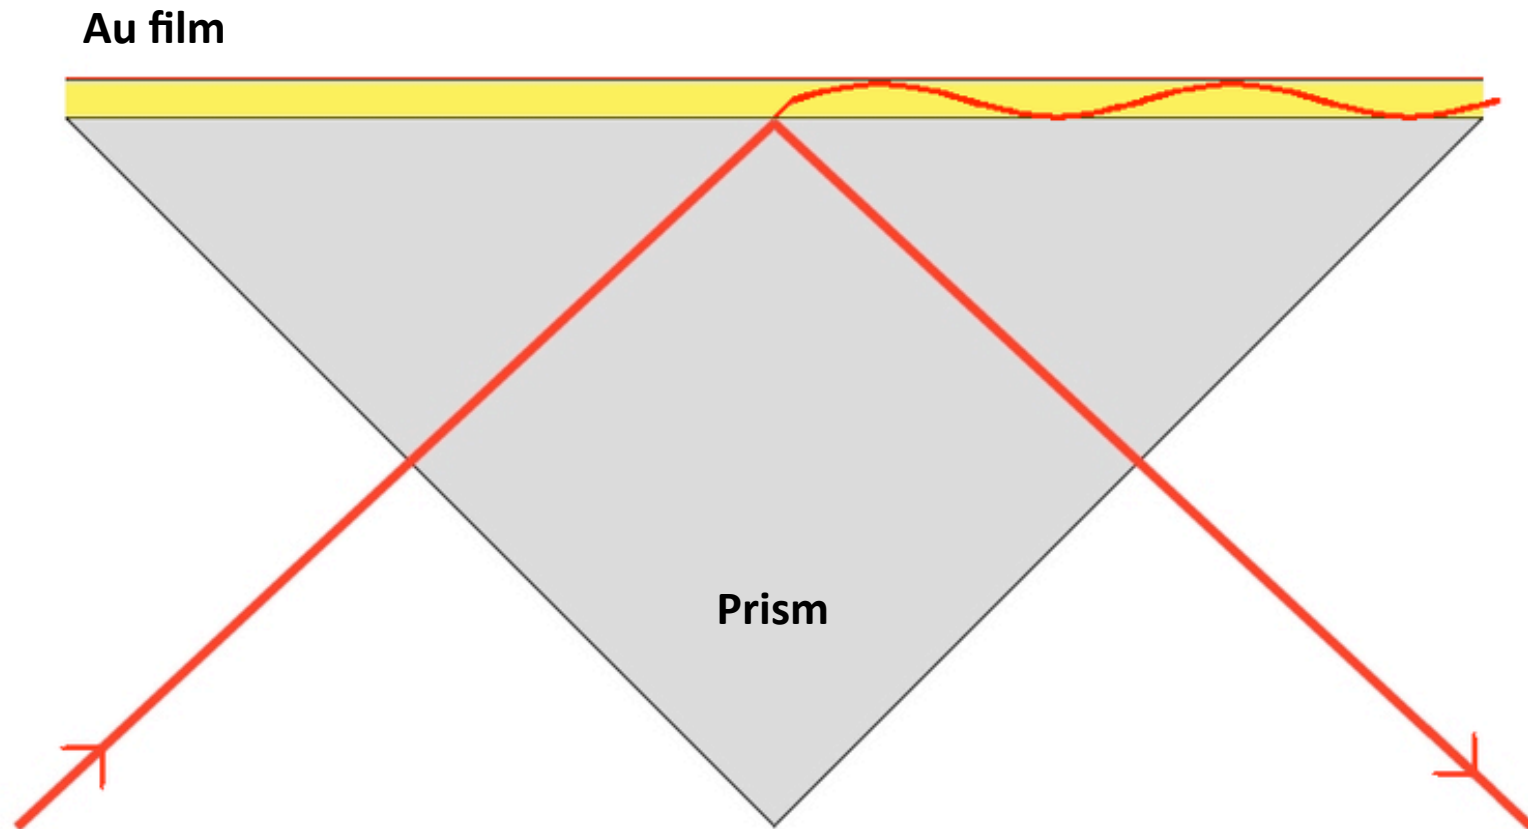


An SPR apparatus and its schematic representation

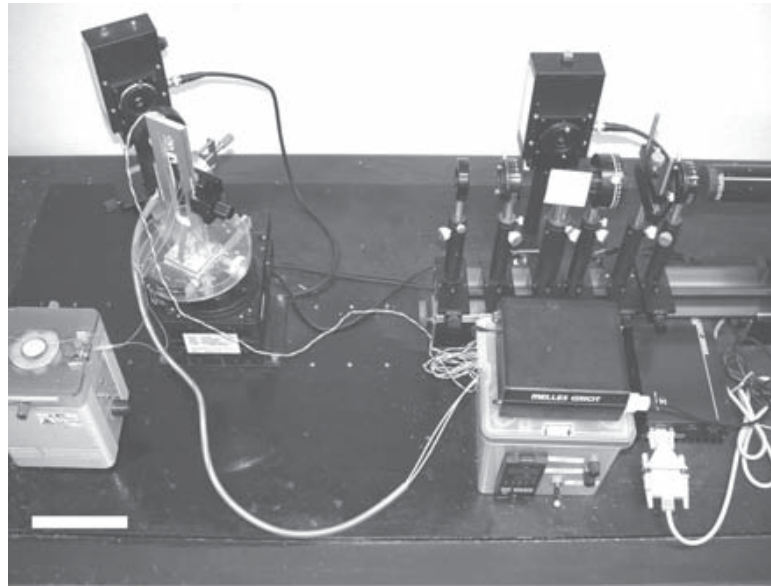


A Rasooly and K E Herold (eds.),
*Methods in Molecular Biology:
Biosensors and Biodetection, Vol.
503*

DOI: [10.1007/978-1-60327-567-5_1](https://doi.org/10.1007/978-1-60327-567-5_1)

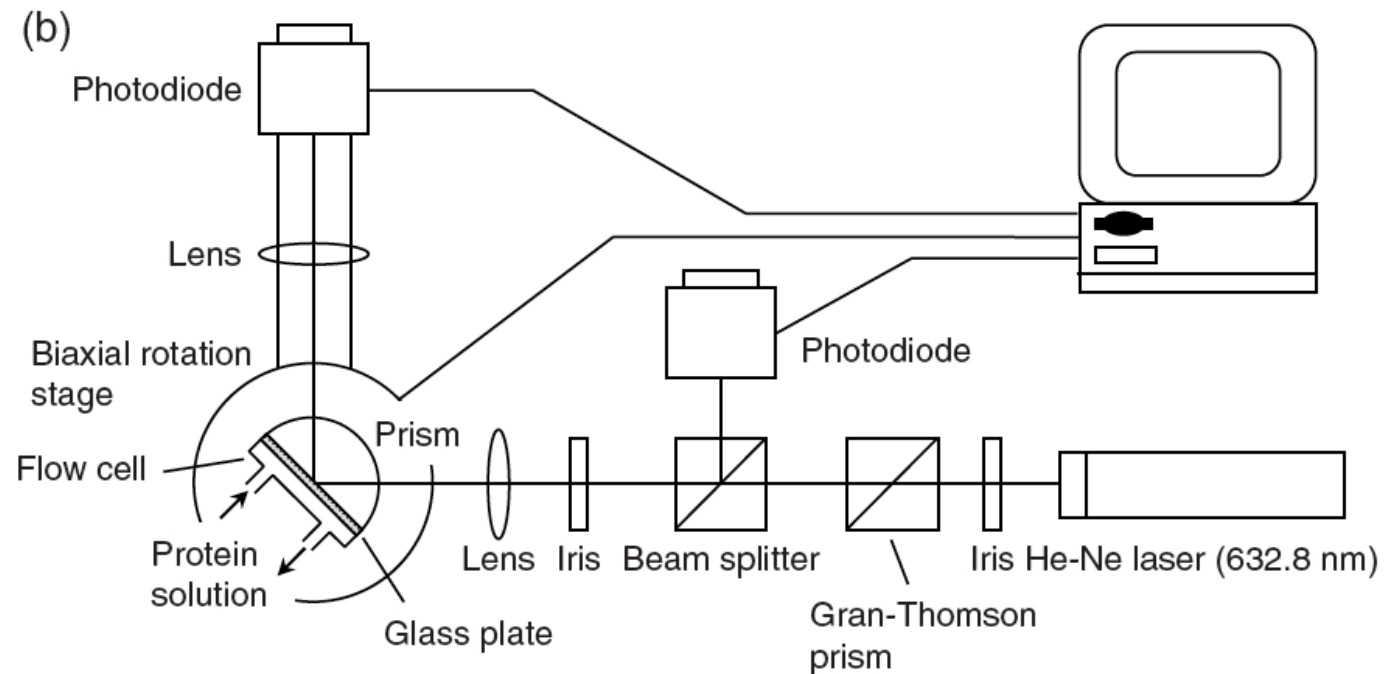


SPR sensor

(a)

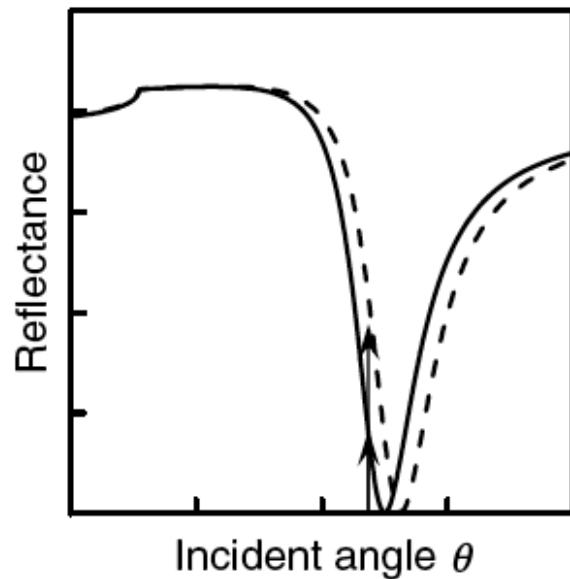

(b)

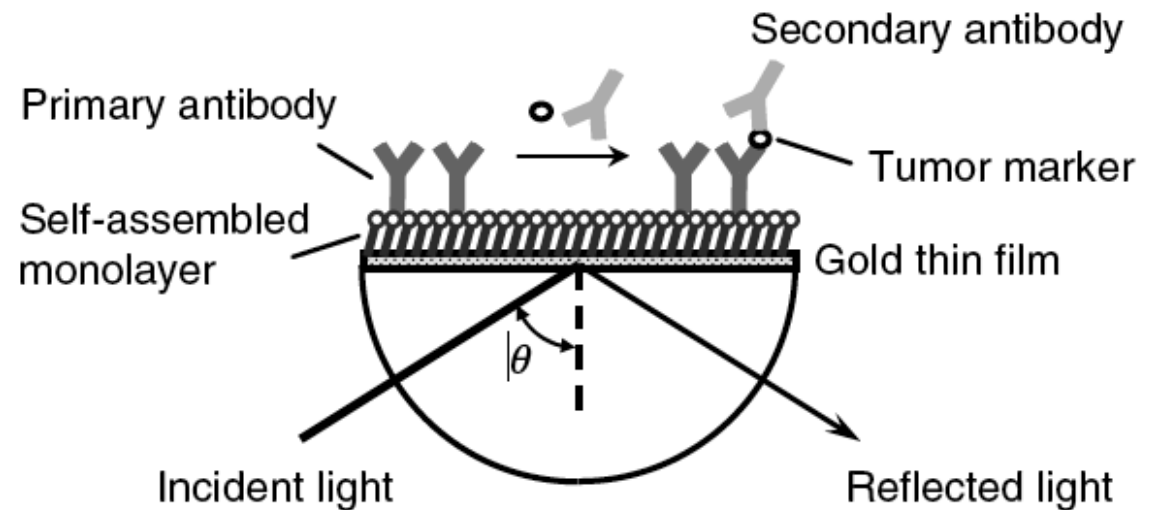


(a) Relationship between incident angle θ and intensity of reflected light before (solid line) and after (dashed line) protein adsorption. For real-time monitoring, the intensity of reflected light is monitored at a fixed angle throughout the measurement (arrow).

(b) Schematic representation of SPR-based sandwich-type immunoassay.




Signal amplification methods for detection of a minute amount of tumor marker


(a)

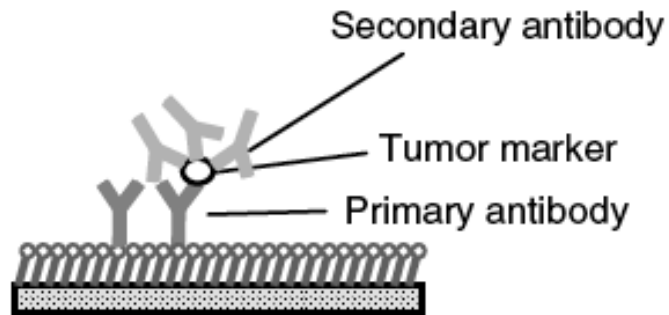


(b)

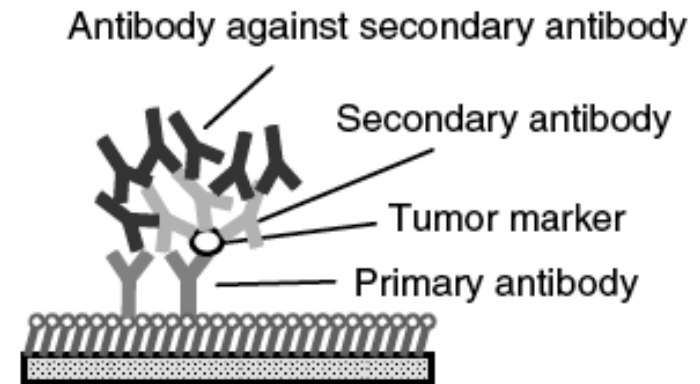


(c)

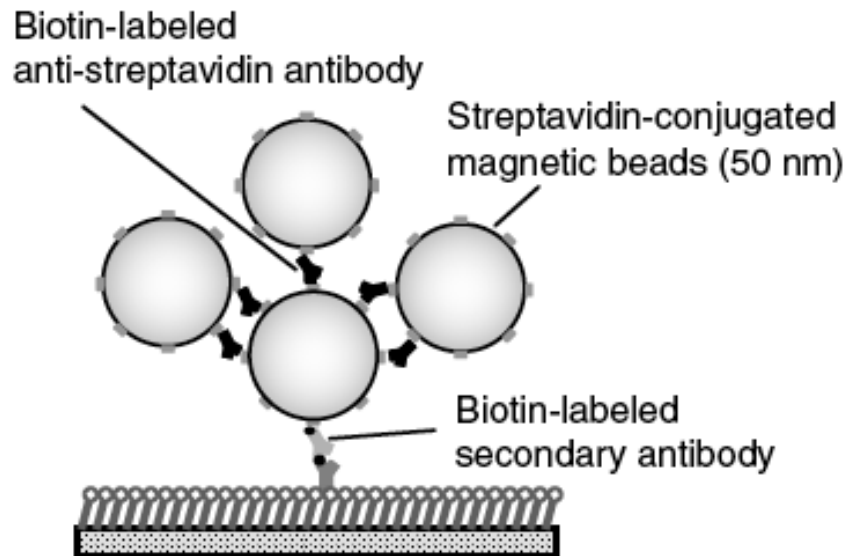

(d)

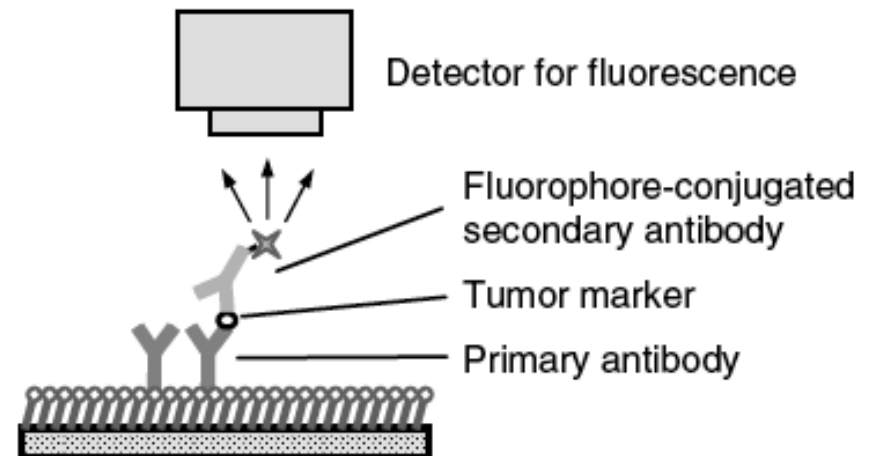


SPR-adsorption-data

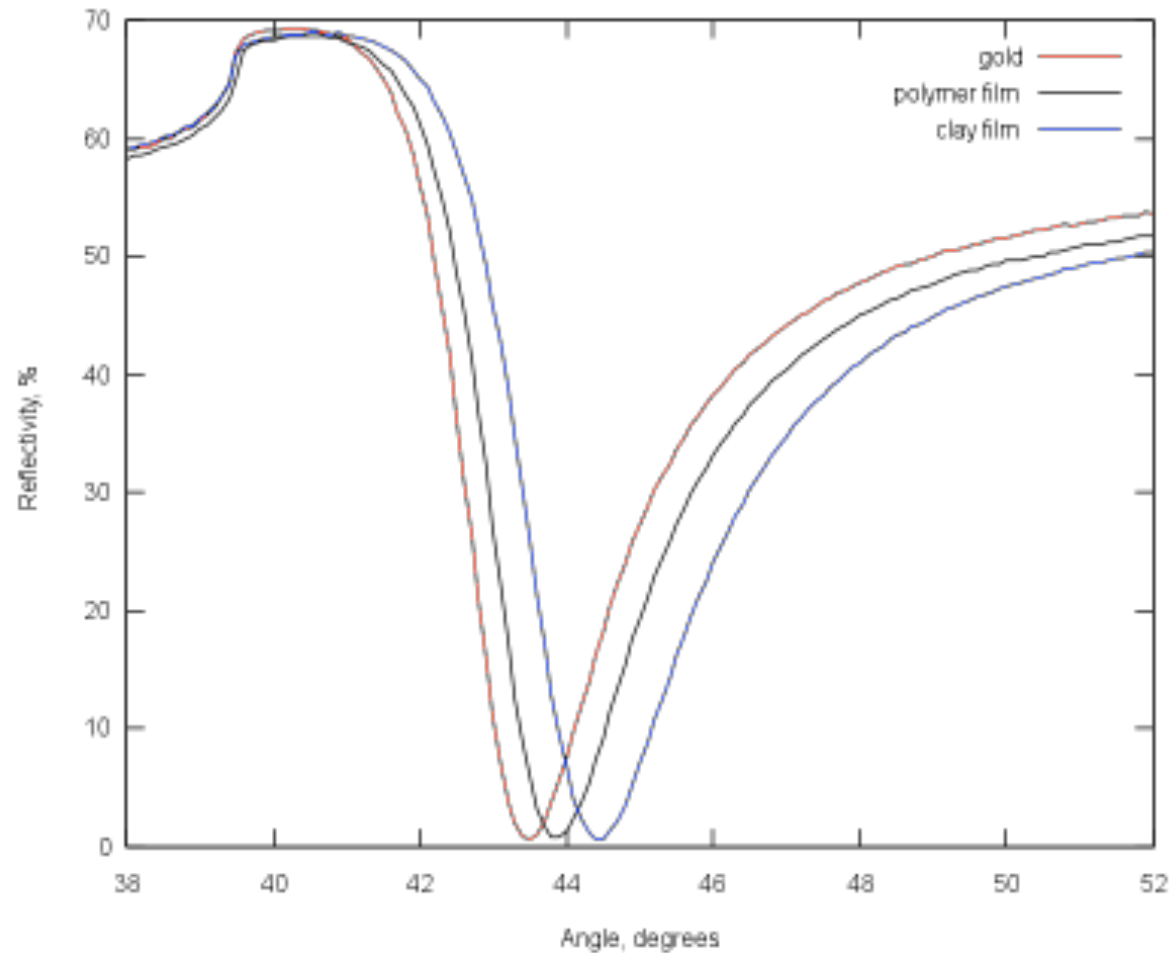

SPR data measured during layer-by-layer self-assembly of PDDACI and Na-montmorillonite clay on gold nanofilm (ca. 38 nm thick). Measurement data from Tamas Haraszti (at that time Department of Colloid Chemistry, University of Szeged, 1997)


Biocore SPR sensor platform

Using the surface plasmon resonance (SPR) phenomenon

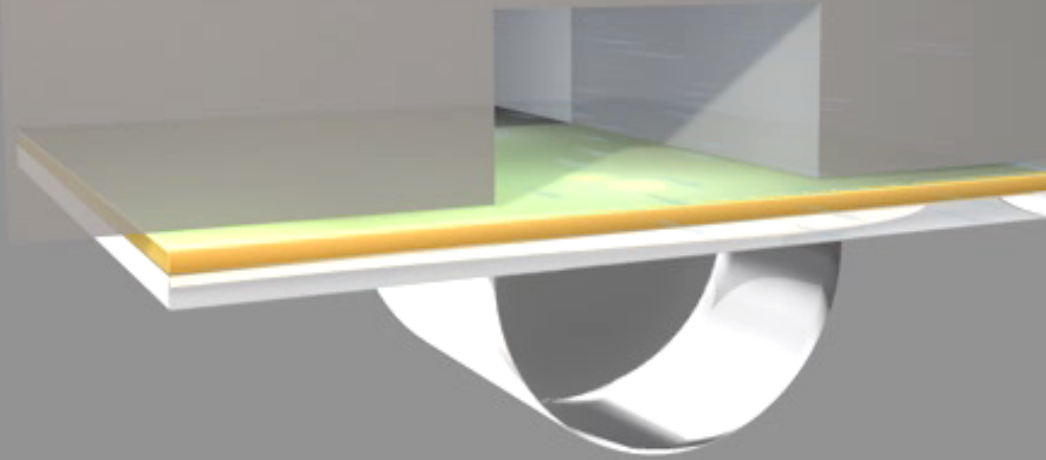


© Biacore AB 2005 a GE Healthcare company


Biocore SPR sensor platform

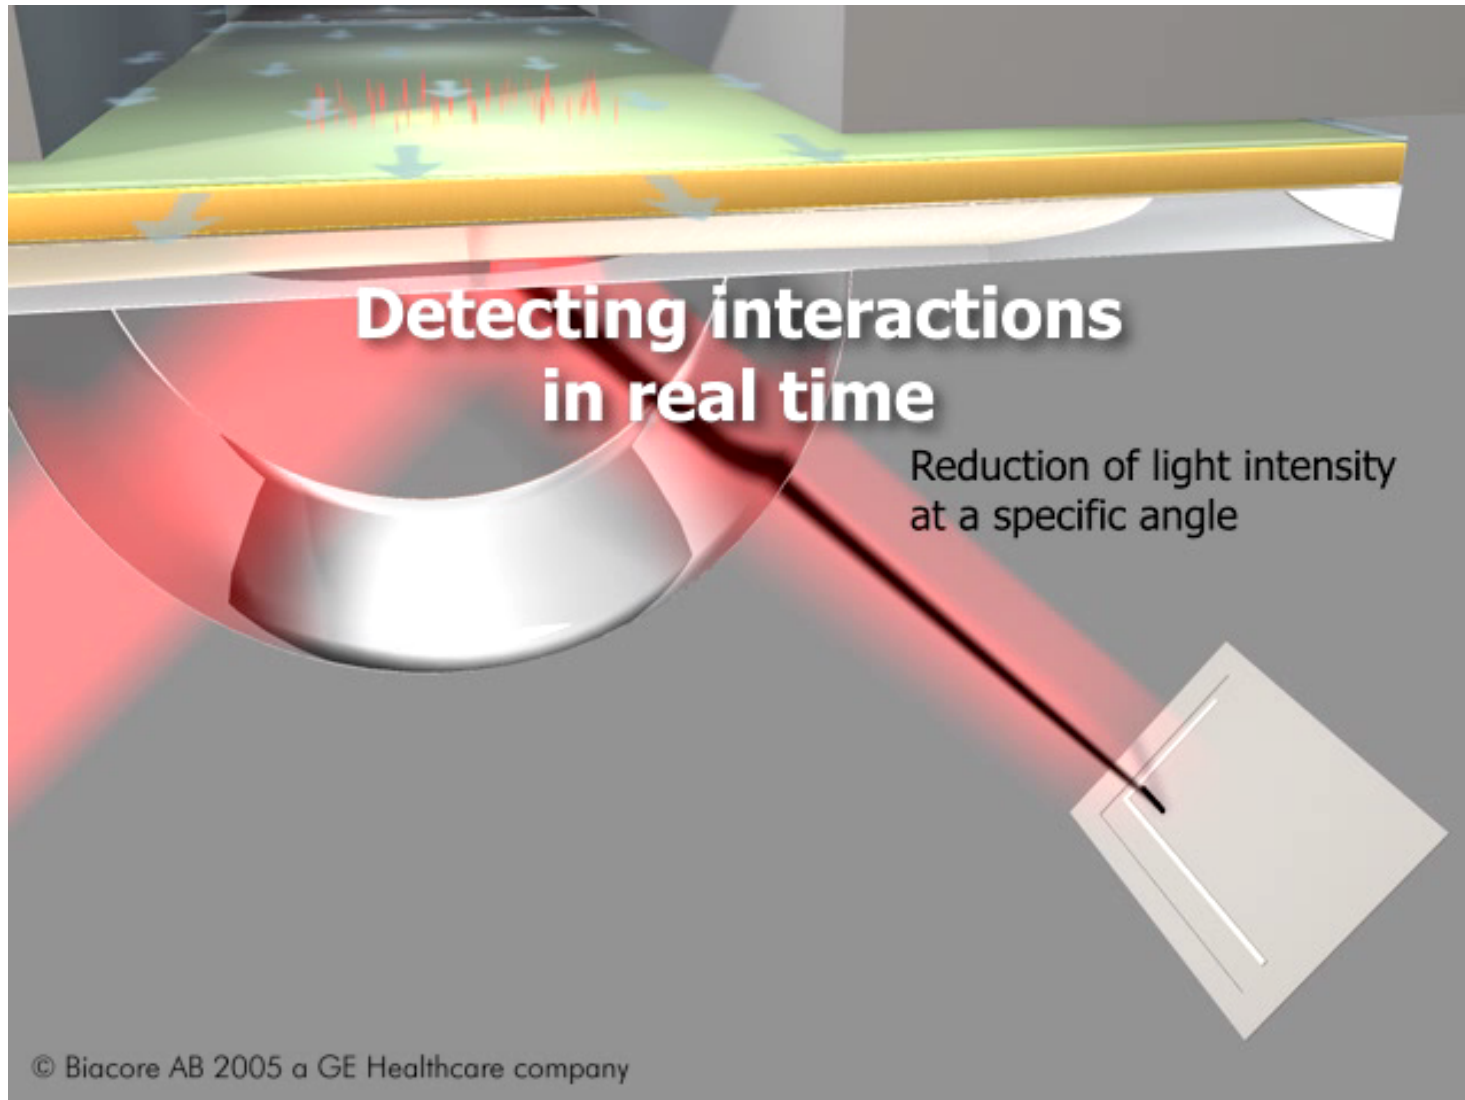

Biocore SPR sensor platform-Kinetics

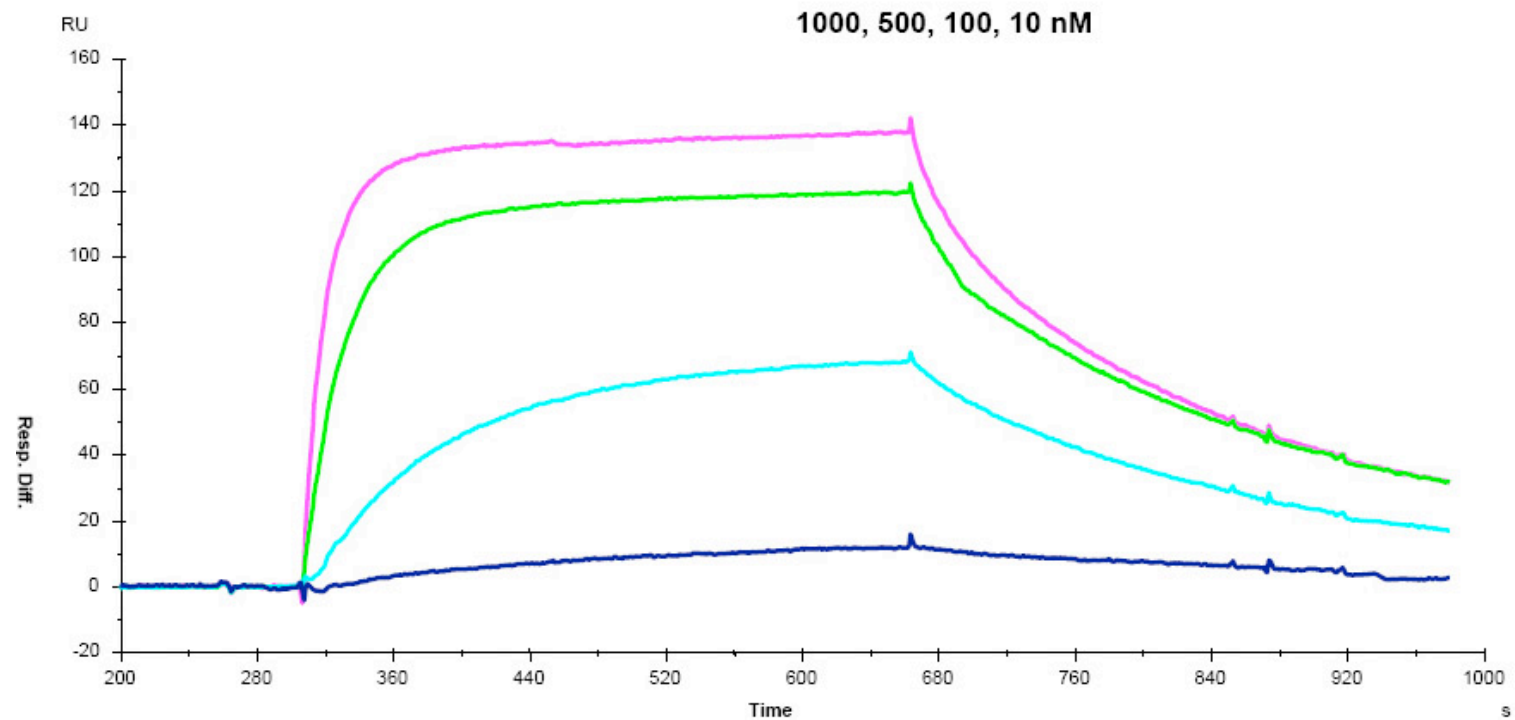

The Sensorgram

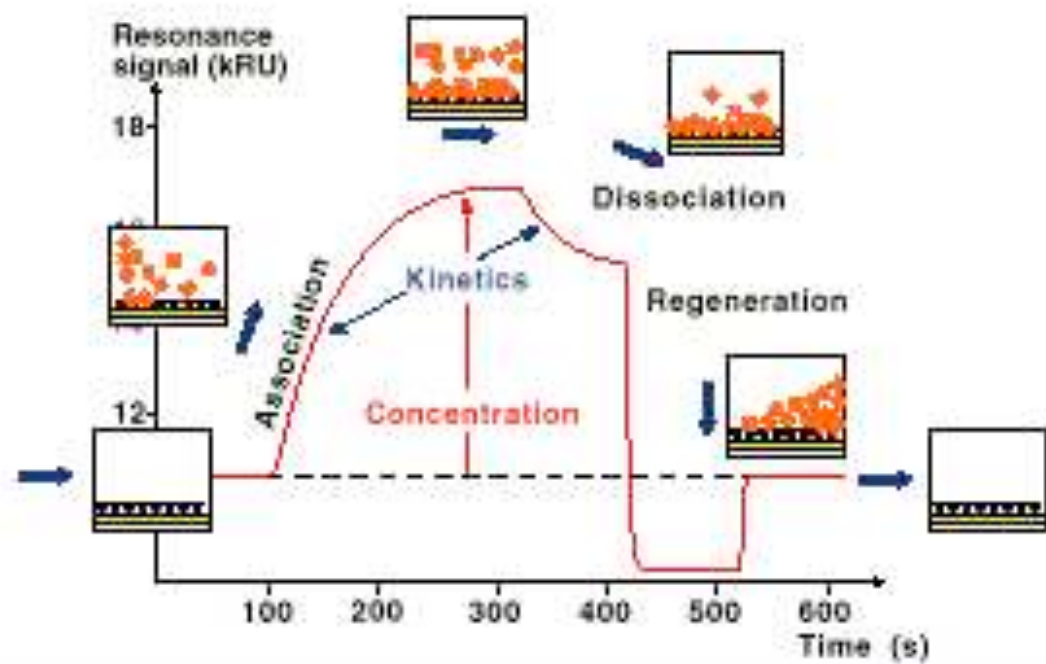



Raman Spectroscopy (SERS)

Why SERS


Sensitive, signals as molecular fingerprints, no photo-bleaching

Current method

Ag/Au colloidal particles, core-shell colloids, roughened Ag films (SERGen)

Open Questions


No compatibility with microfabrication,
No integration with microfluidic
Devices, un-repeatable enhancement
factor

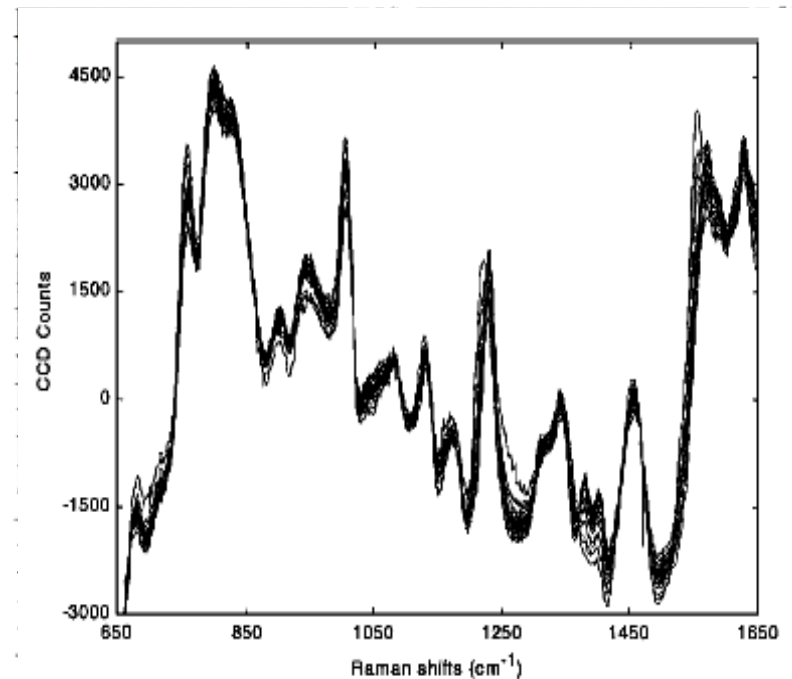


Raman Spectroscopy

ECM SNP Detection


Electrochemical detection

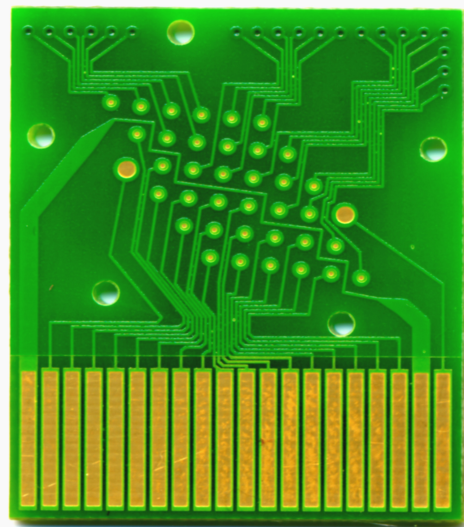


eSensor™
DNA DETECTION TECHNOLOGY
Making DNA testing a routine part of medicine and industry

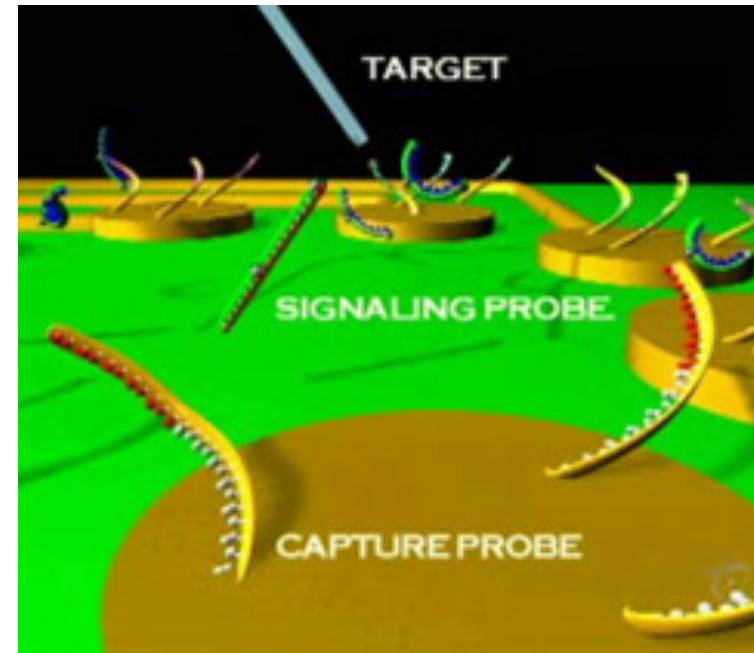

Use of 2 probes = double specificity


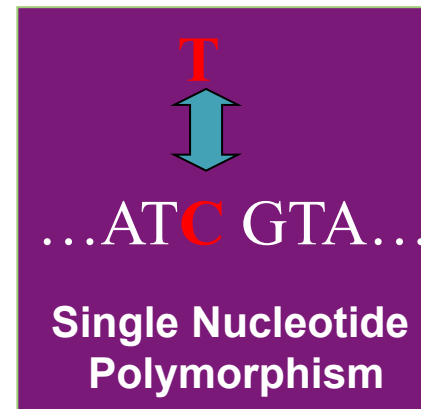


ECM SNP Detection

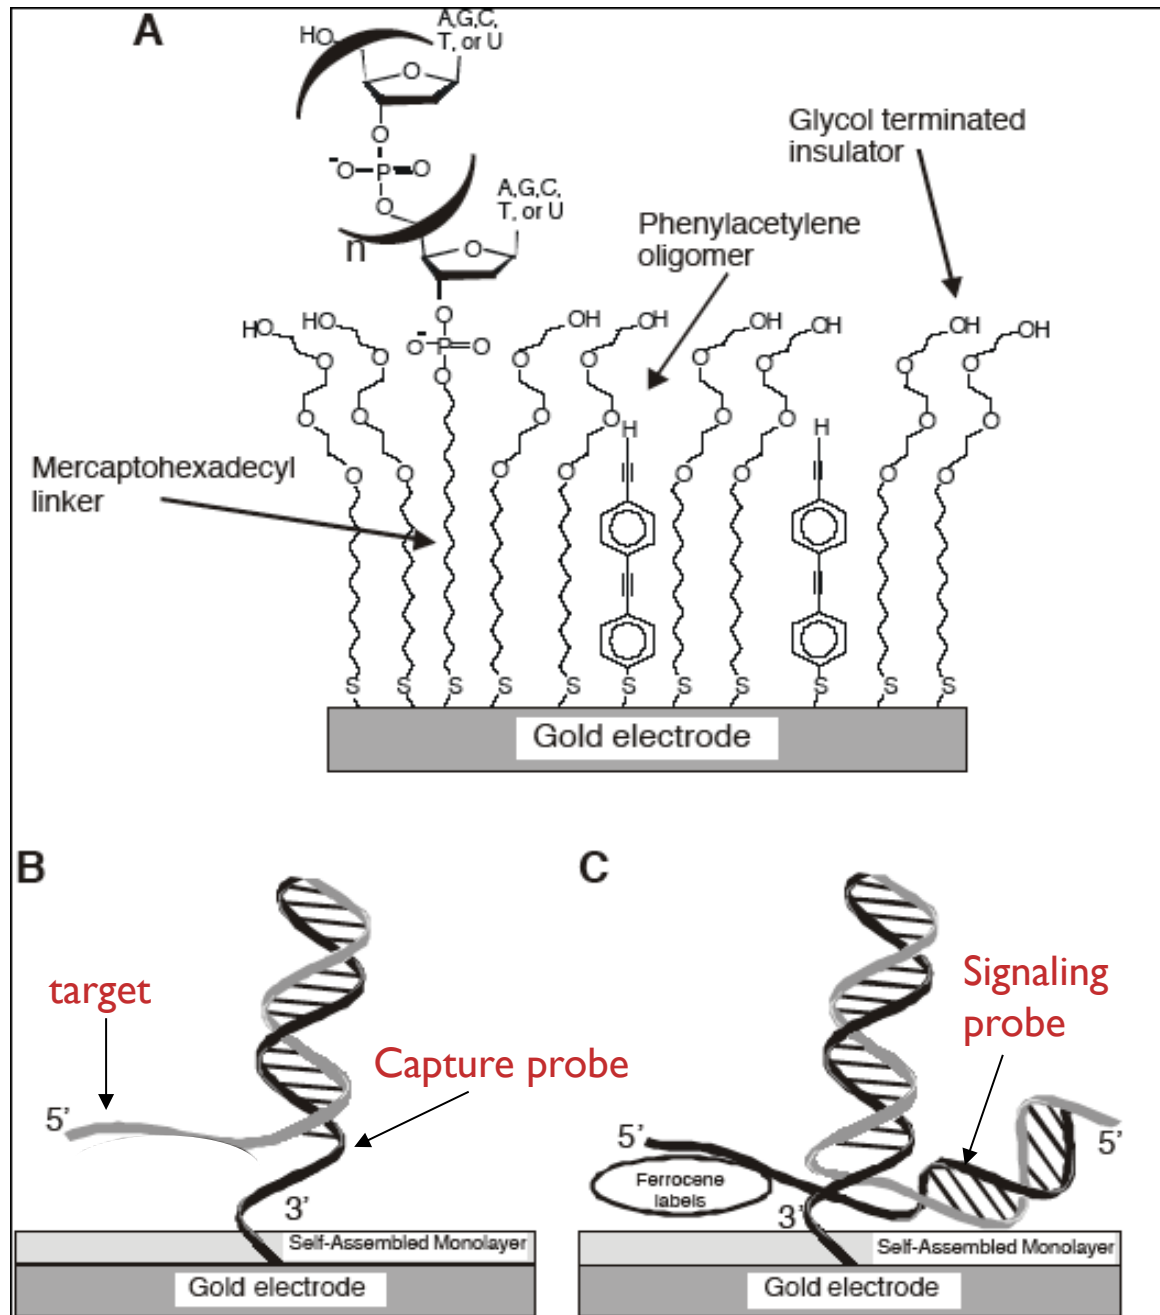

Umek, R. M.; et al. Electronic Detection of Nucleic Acids: A Versatile Platform for Molecular Diagnostics. *J. Mol. Diagn.* 2001, 3, 74.

ACV detection of DNA hybridization events

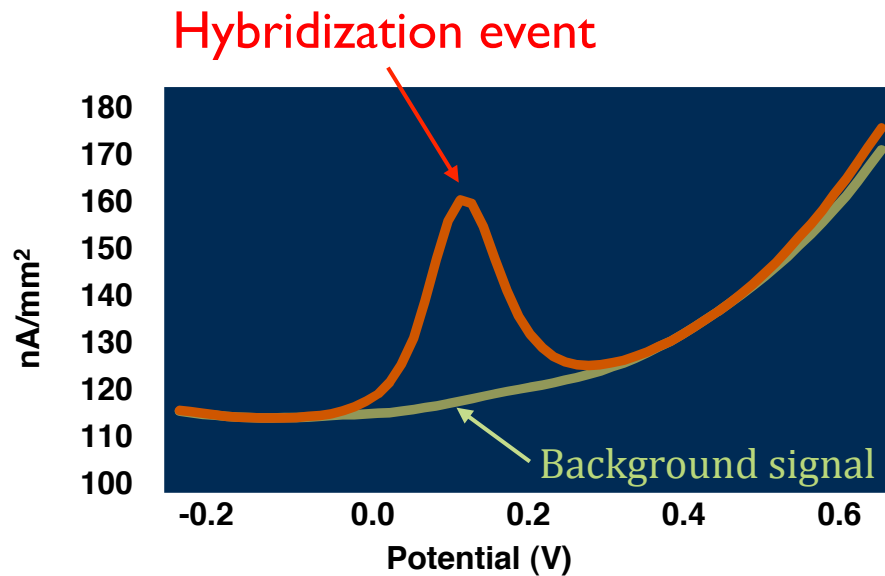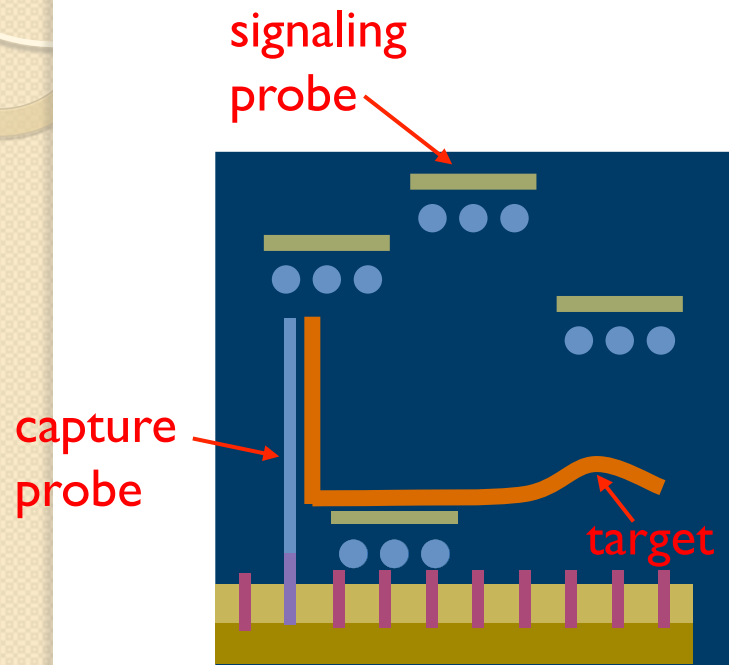


Umek, R. M.; et al. Electronic Detection of Nucleic Acids: A Versatile Platform for Molecular Diagnostics. *J. Mol. Diagn.* 2001, 3, 74.


NS Swami, CF Chou, and R Terberueggen. Two-Potential Electrochemical Probe for Study of DNA Immobilization. *Langmuir* 2005, 21, 1937-1941.

Cross section of an n-type MOSFET

(metal oxide semiconductor field effect transistor)






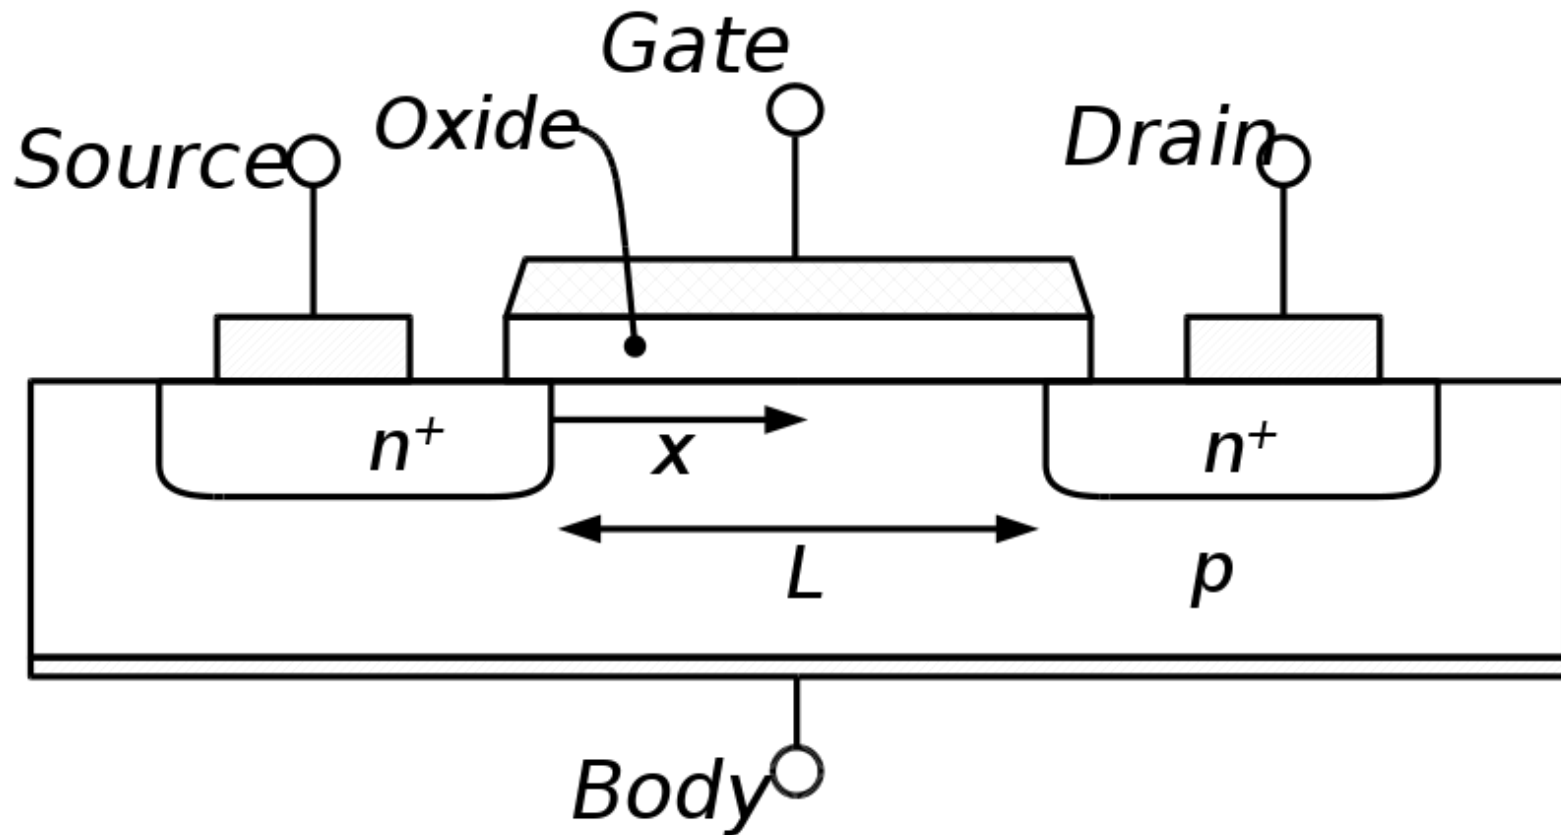


Field effect transistors (FETs) as transducers in electrochemical sensors

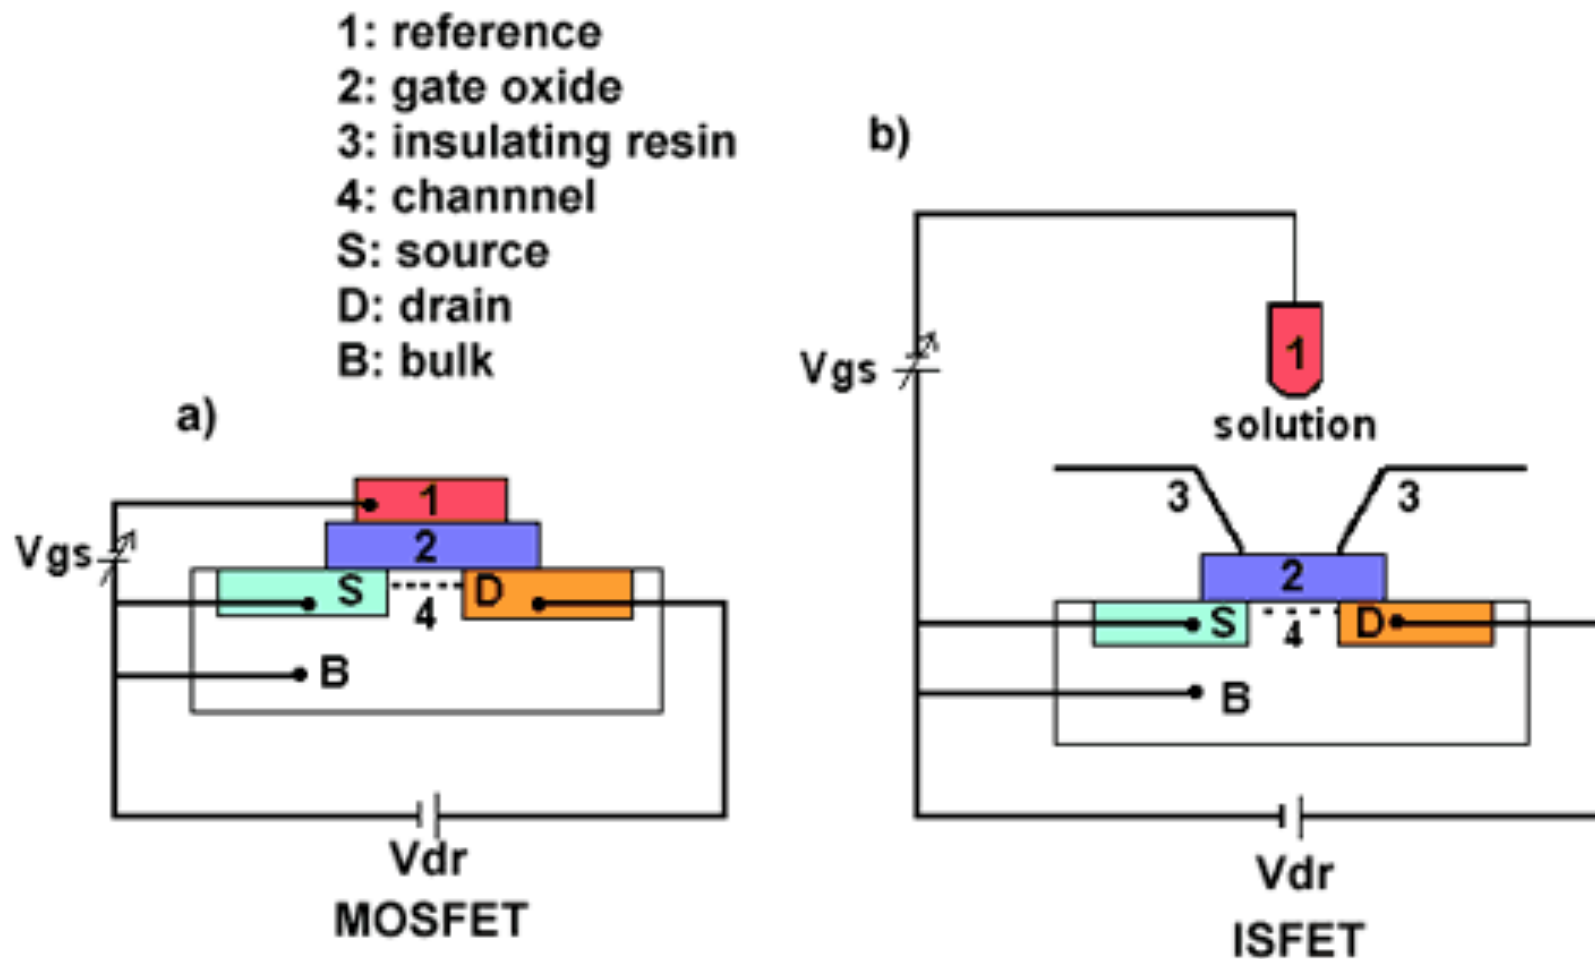


Nanowire sensor array

Zheng GF, Patolsky F, Cui Y, et al. Multiplexed electrical detection of cancer markers with nanowire sensor arrays. *NAT BIOTECH* 23, 1294-1301 (2005).

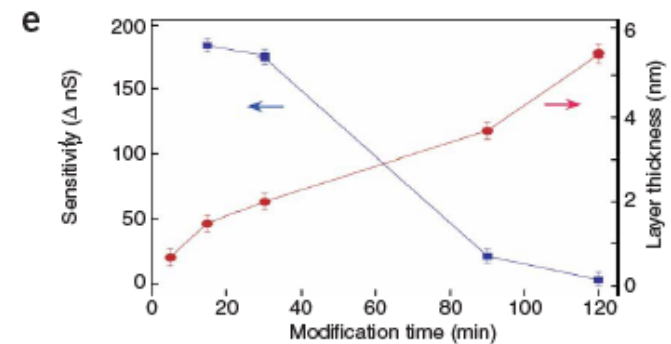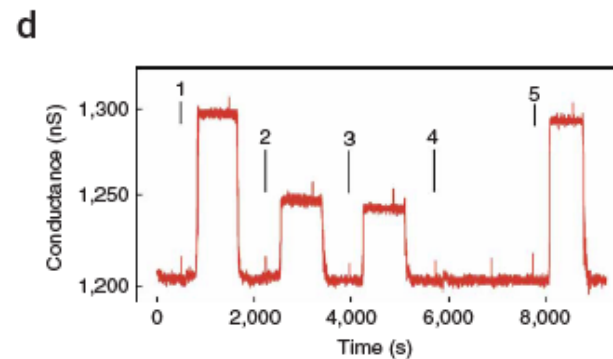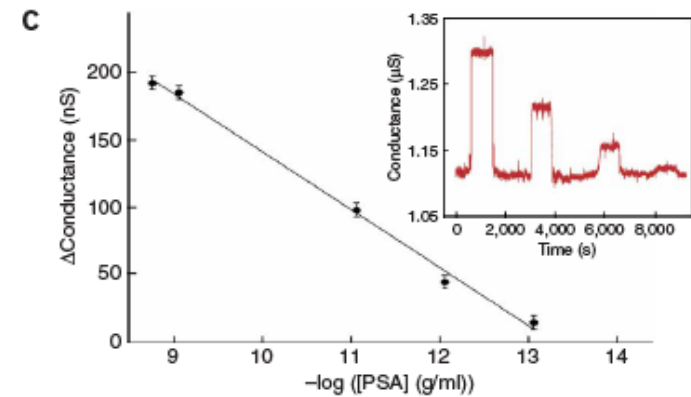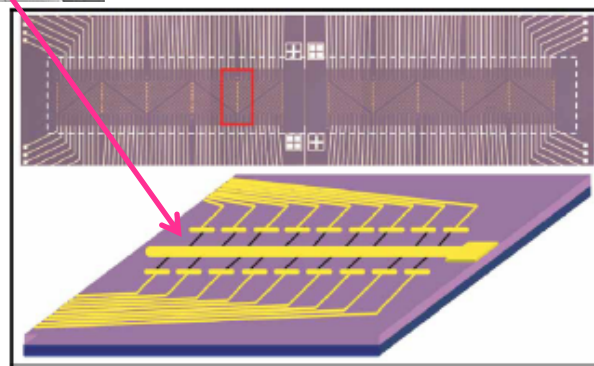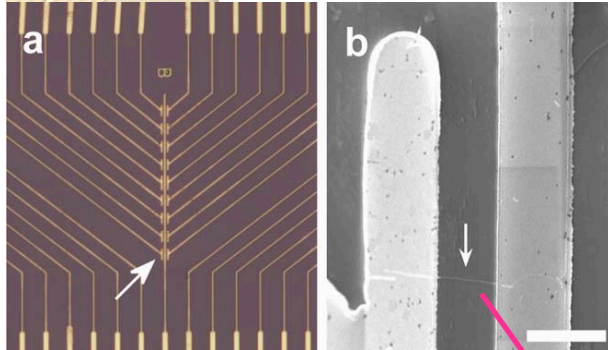


Biosensors Based on Cantilevers

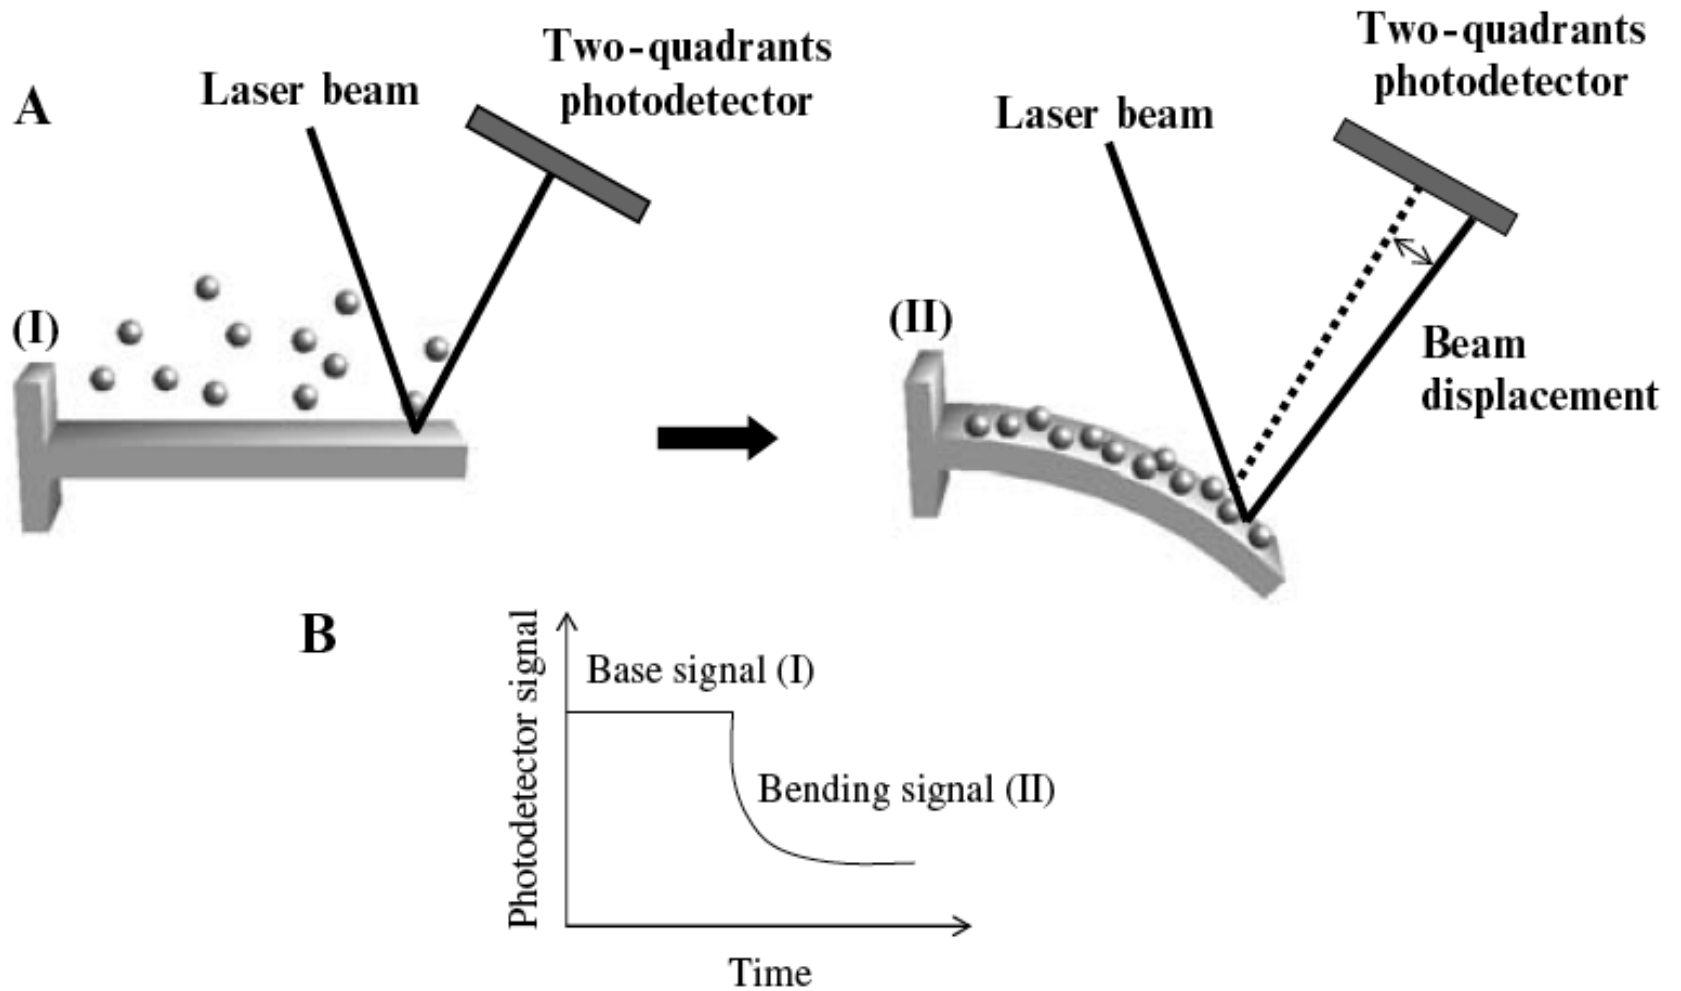




Cantilever surface functionalization in real time


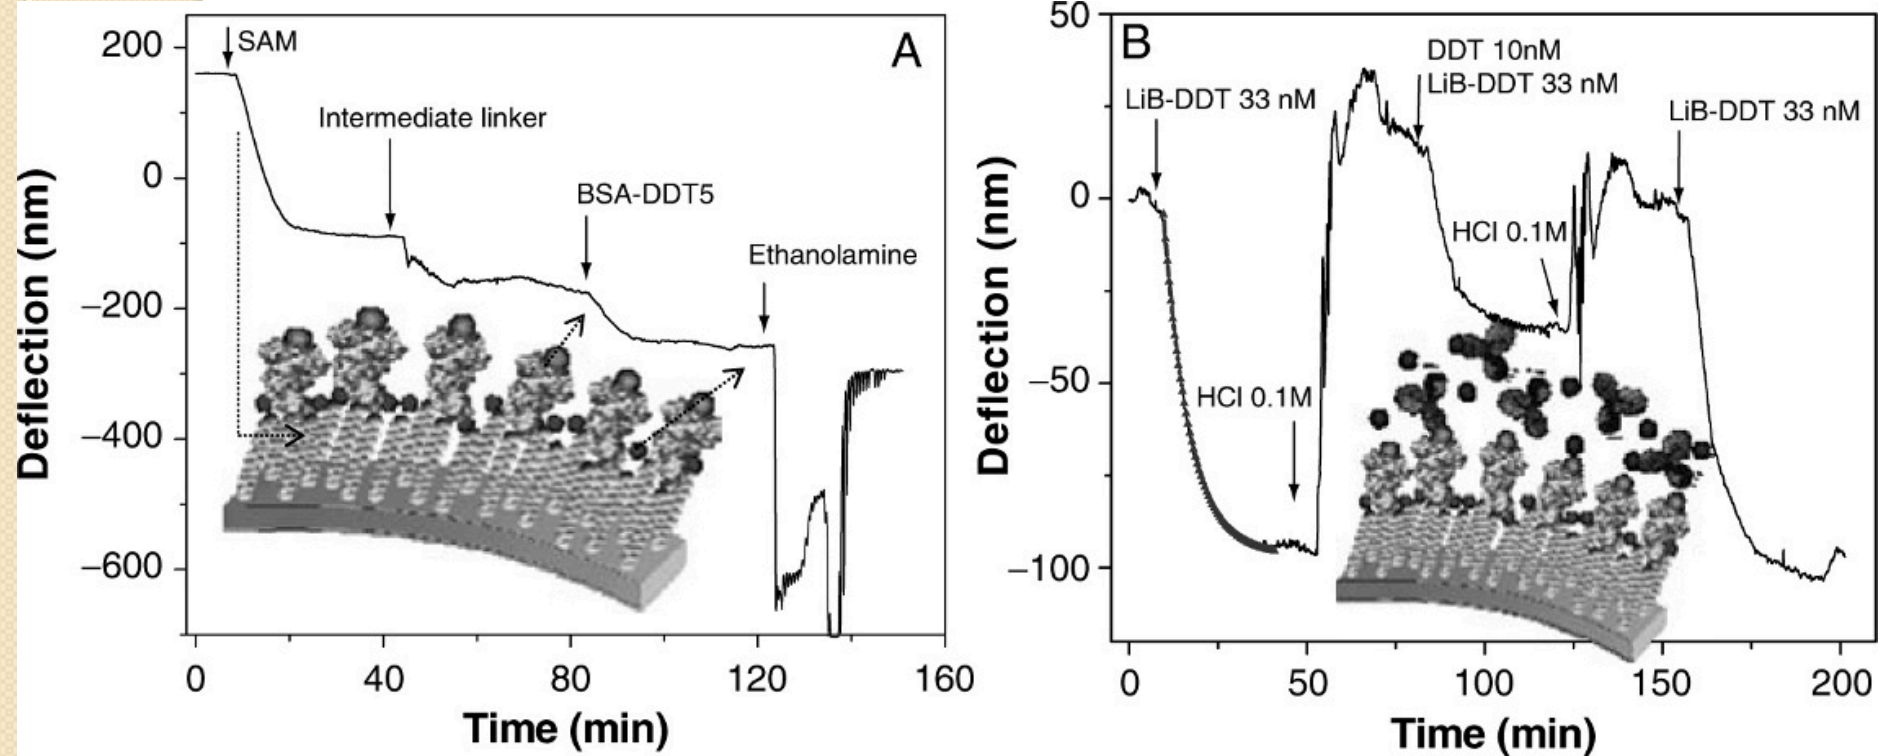


(A) Example of a cantilever surface functionalization in real time. Each one of the layers formed over the surface produce a cantilever bending. (B) Real-time monitoring of an antibody direct detection and a competitive immunoassay. The number of antibodies free in solution able to binding the cantilever surface is reduced due to the binding with the DDT free in solution. The cantilever surface was regenerated with 100 mM HCl (100 ml) to break the hapten/antibody complex; (M. Alvarez et al. (2003) Development of nanomechanical biosensors for detection of the pesticide DDT. *Biosen. Bioelectron.* 18, 649–653).

Integrated Genetic Analysis System

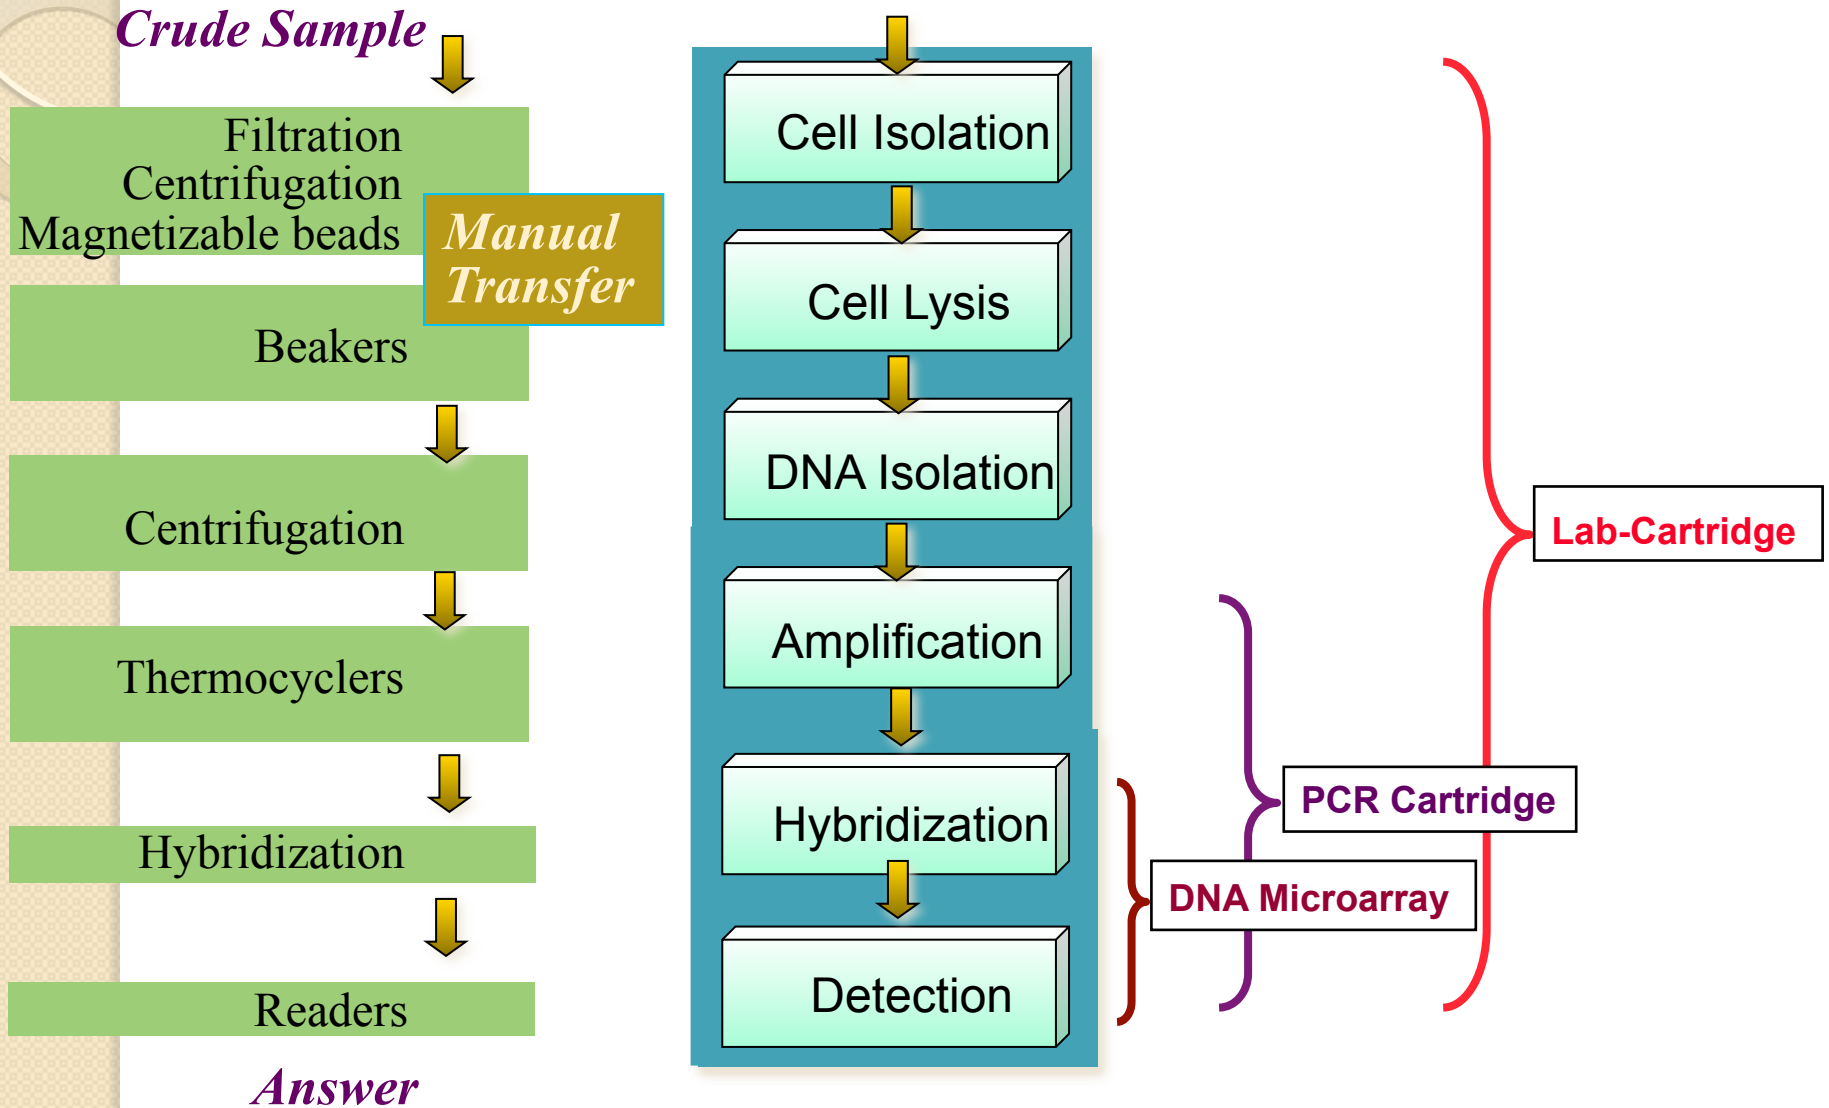


Integrated Genetic Analysis System

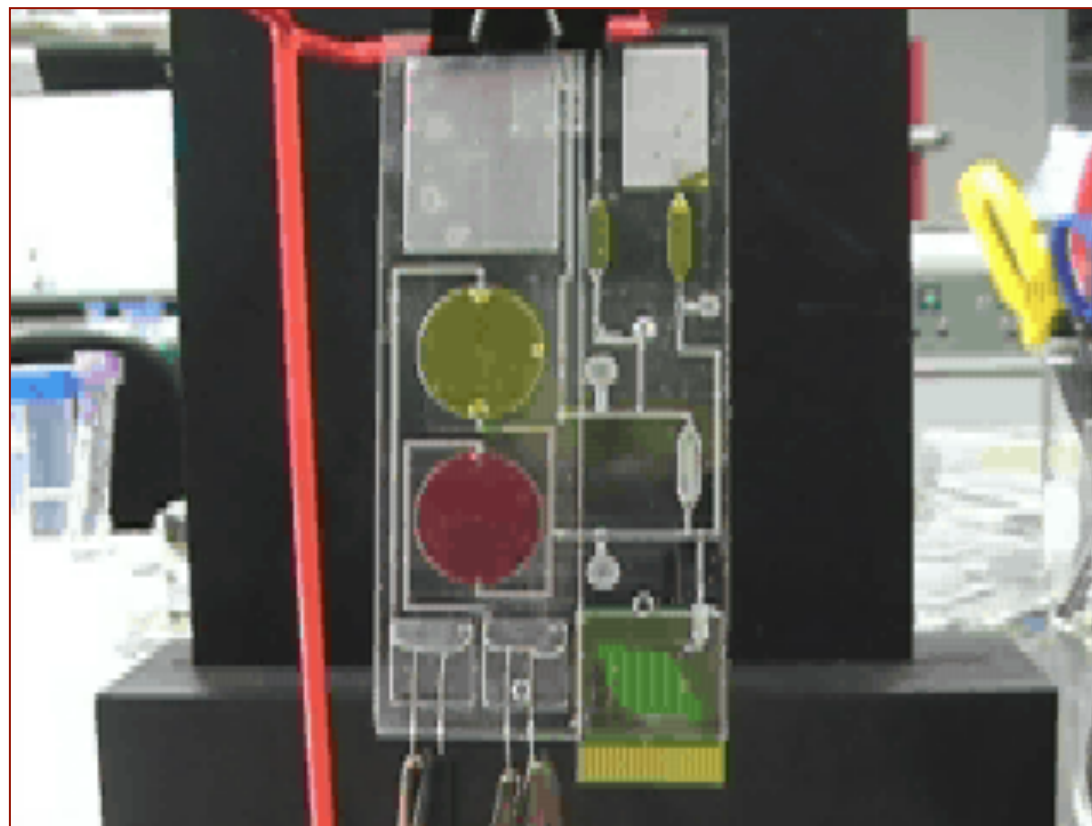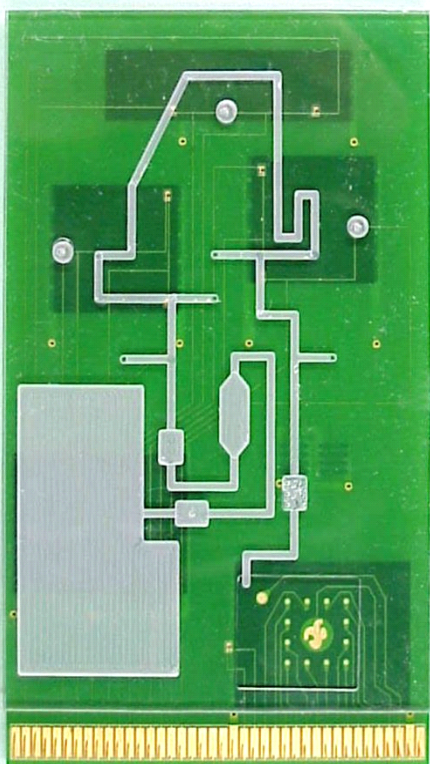

RH Liu et al. ANAL. CHEM. 76, 1824 (2004)

Real-time Single Molecule Sequencing

Helicos platform

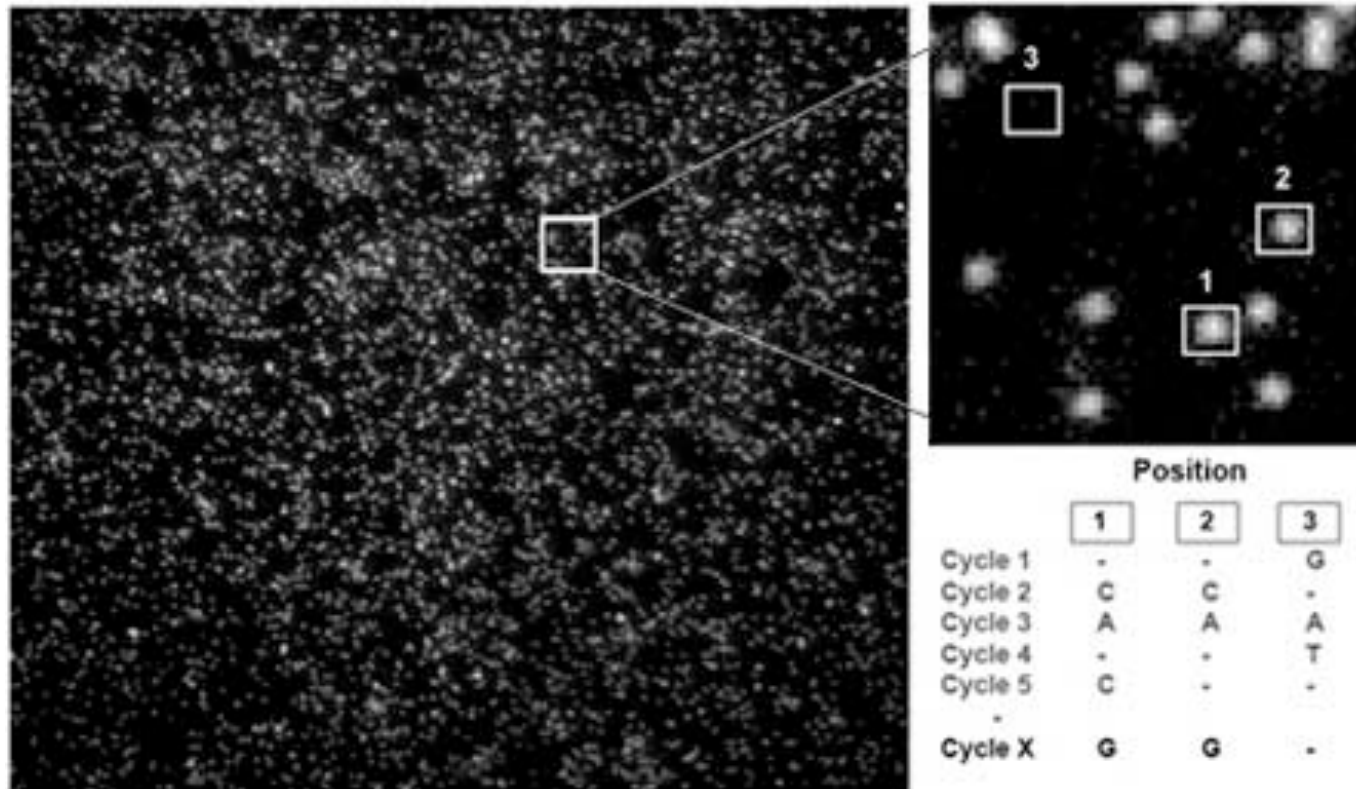

<http://www.helicosbio.com/>




Zero-Mode Waveguides for Single-Molecule Analysis at High Concentrations

Science 299, 682-686, 2003


M. J. Levene,¹ J. Korlach,^{1,2} S. W. Turner,^{1*} M. Foquet,¹
H. G. Craighead,¹ W. W. Webb^{1†}

Optical approaches for observing the dynamics of single molecules have required pico- to nanomolar concentrations of fluorophore in order to isolate individual molecules. However, many biologically relevant processes occur at micromolar ligand concentrations, necessitating a reduction in the conventional observation volume by three orders of magnitude. We show that arrays of zero-mode waveguides consisting of subwavelength holes in a metal film provide a simple and highly parallel means for studying single-molecule dynamics at micromolar concentrations with microsecond temporal resolution. We present observations of DNA polymerase activity as an example of the effectiveness of zero-mode waveguides for performing single-molecule experiments at high concentrations.

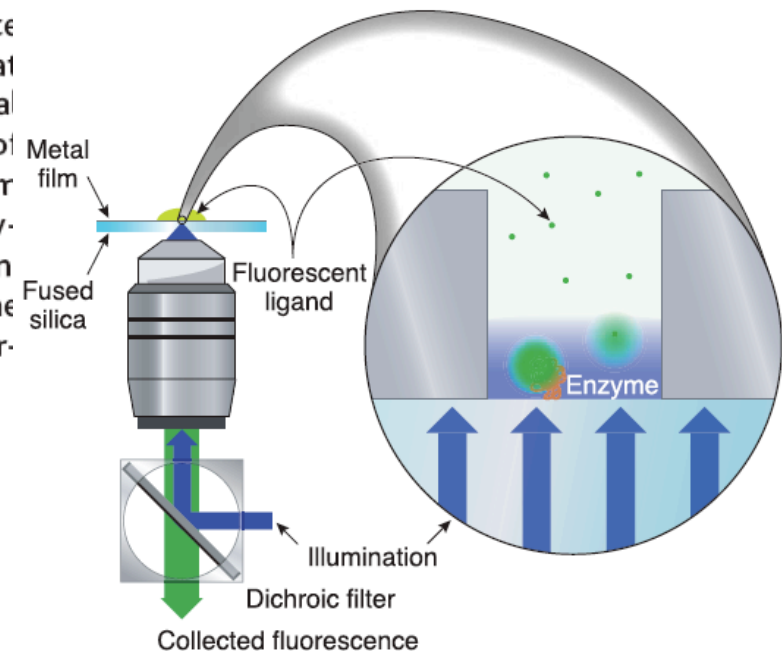

An apparatus for single-molecule enzymology using zero-mode waveguides.

Real-time Single Molecule Sequencing

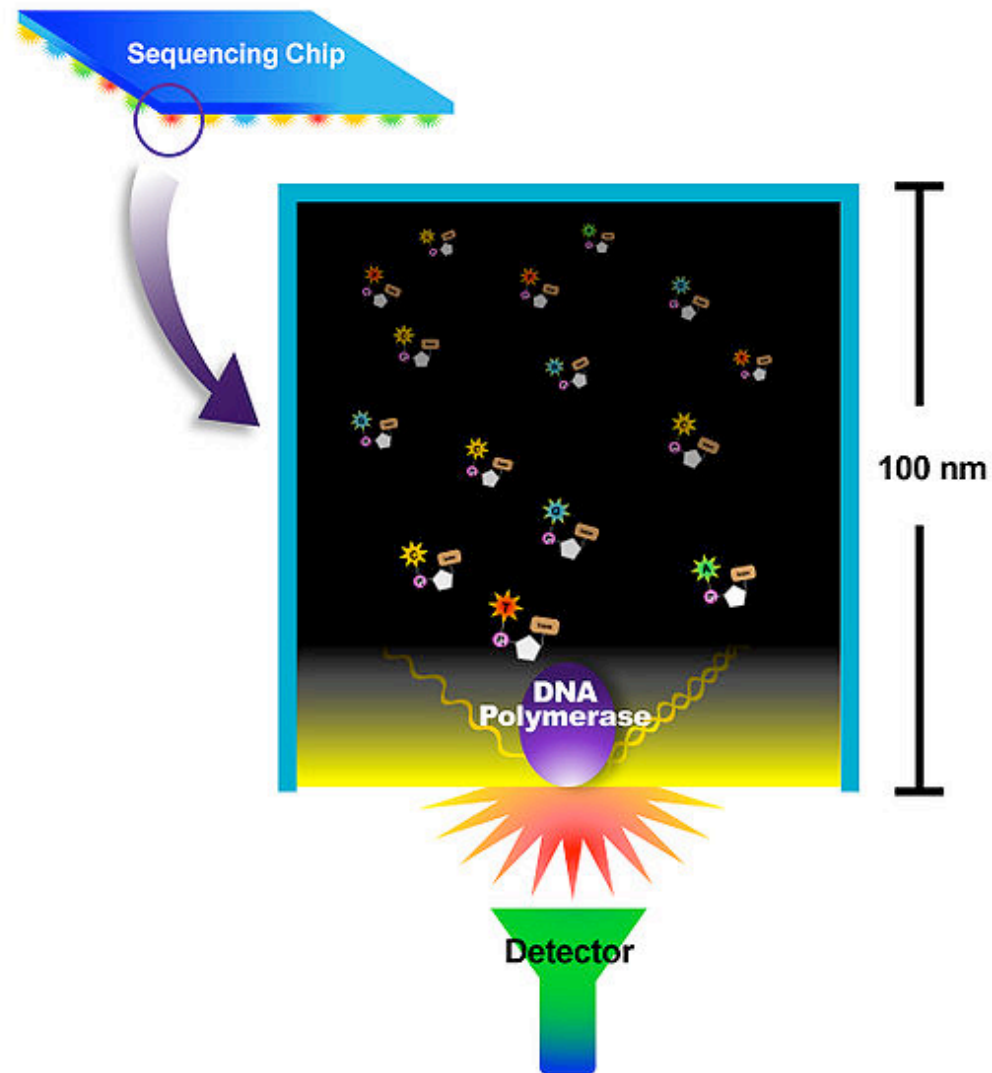



Proc. Natl. Acad. Sci. USA
Vol. 93, pp. 13770–13773, November 1996
Biophysics




Nanopore DNA Sequencing

Characterization of individual polynucleotide molecules using a membrane channel


JOHN J. KASIANOWICZ*, ERIC BRANDIN†, DANIEL BRANTON†‡, AND DAVID W. DEAMER§

*Biotechnology Division, National Institute of Science and Technology, 222/A353, Gaithersburg, MD 20899; †Department of Molecular and Cellular Biology, Harvard University, 16 Divinity Avenue, Cambridge, MA 02138; and ‡Department of Chemistry and Biochemistry, University of California, Santa Cruz, CA 95064


A single α -hemolysin channel ($\varnothing = 1.5$ nm) embedded in a lipid bilayer

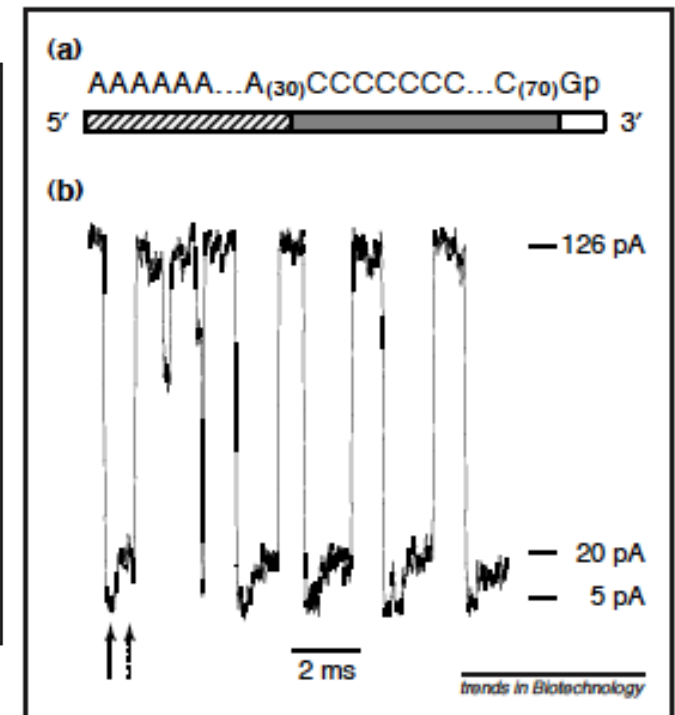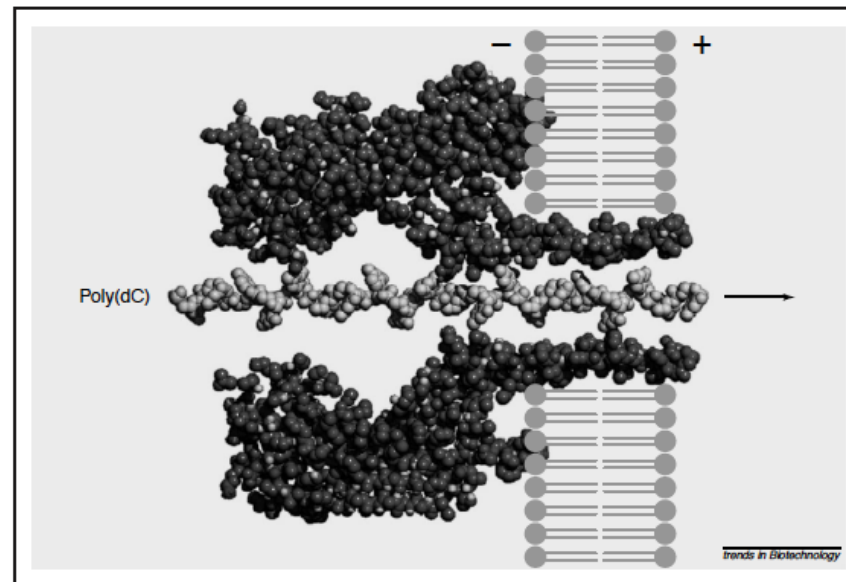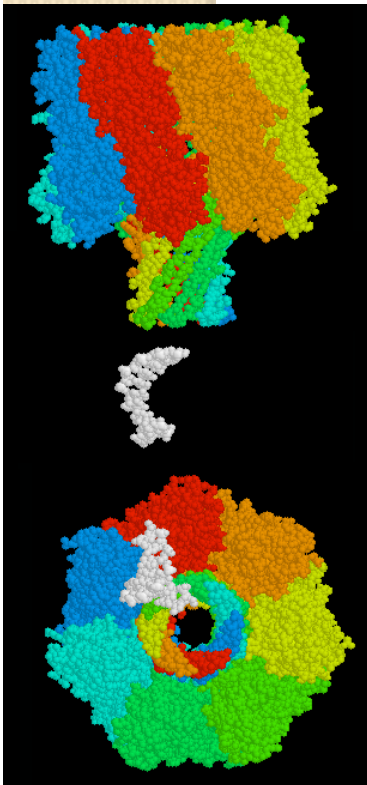


Solid State Nanopore

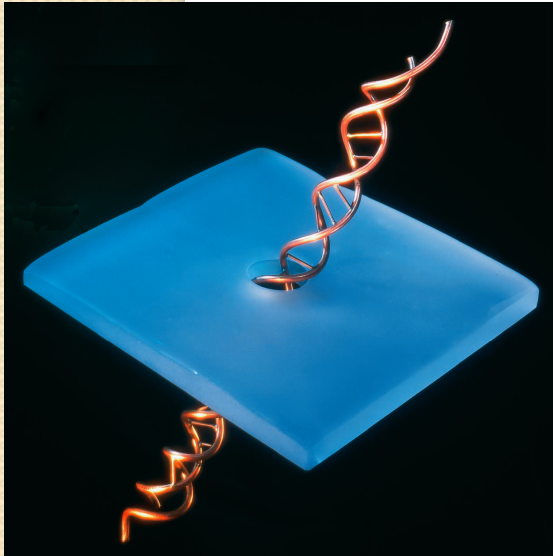

Dekker group, Nat. Mater. 2003

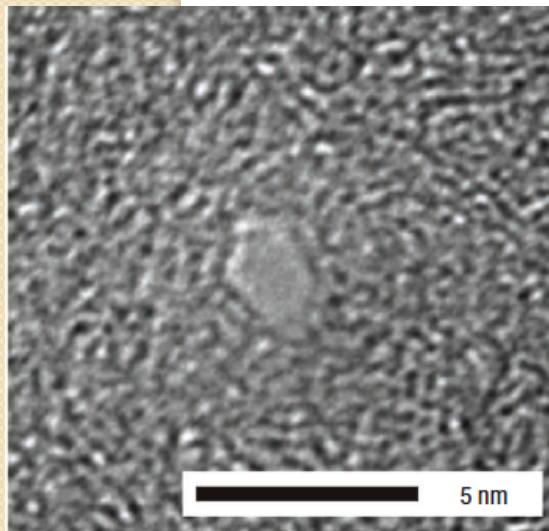

A SOLID STATE NANOPORE
ARTICULATED WITH PROBES

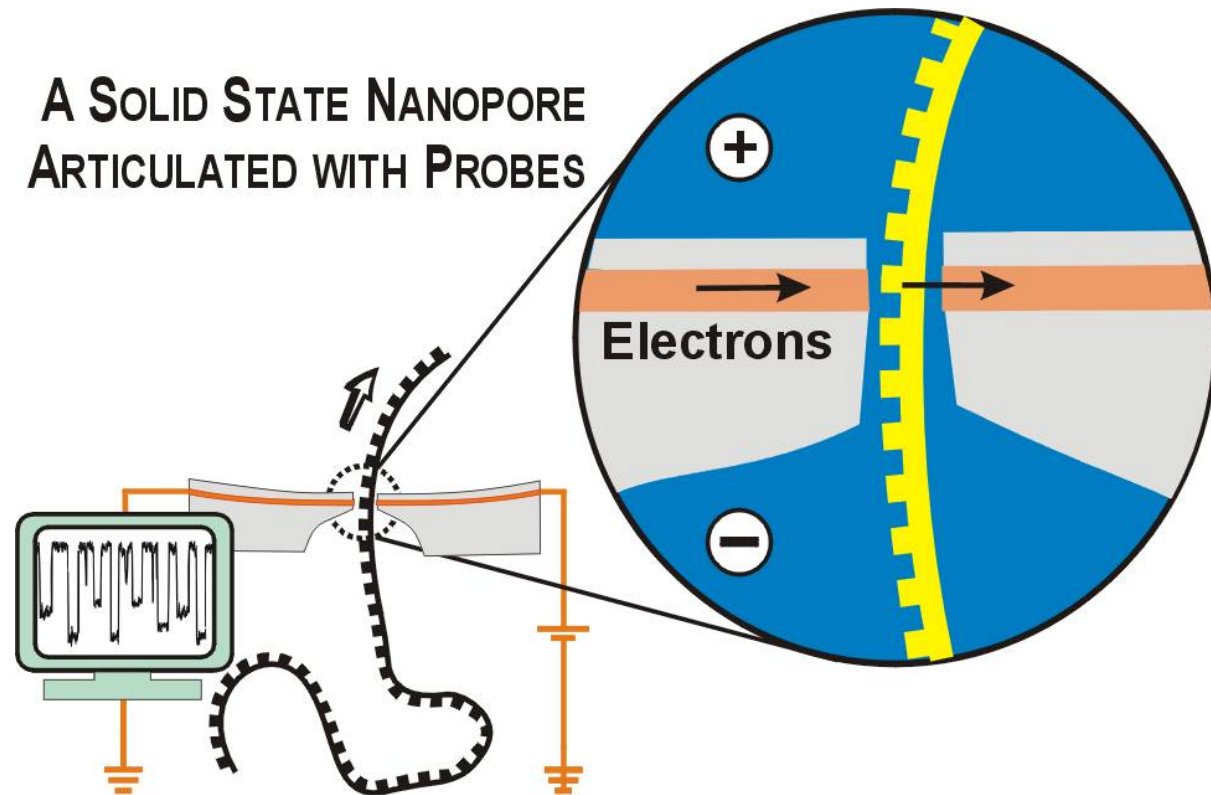


D. Branton, J. Golovchenko, Harvard



The Nobel Prize in Physics 2010

Andre Geim, Konstantin Novoselov

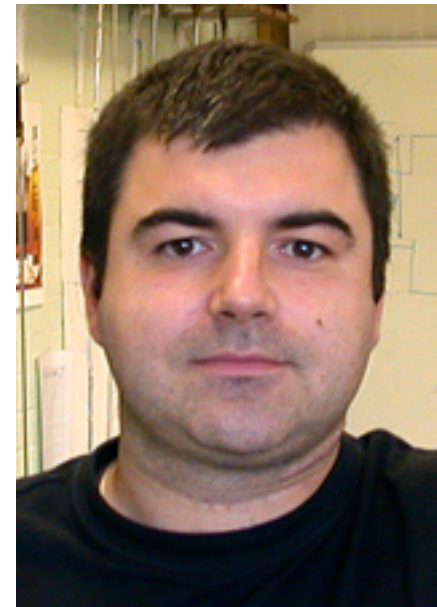

The Nobel Prize in Physics 2010 was awarded jointly to Andre Geim and Konstantin Novoselov *"for groundbreaking experiments regarding the two-dimensional material graphene"*


Title: Electric field effect in atomically thin carbon films

Author(s): Novoselov KS, Geim AK, Morozov SV, et al.

Source: SCIENCE Volume: 306 Issue: 5296 Pages: 666-669 Published: OCT 22 2004

Times Cited: 3,429


Graphene

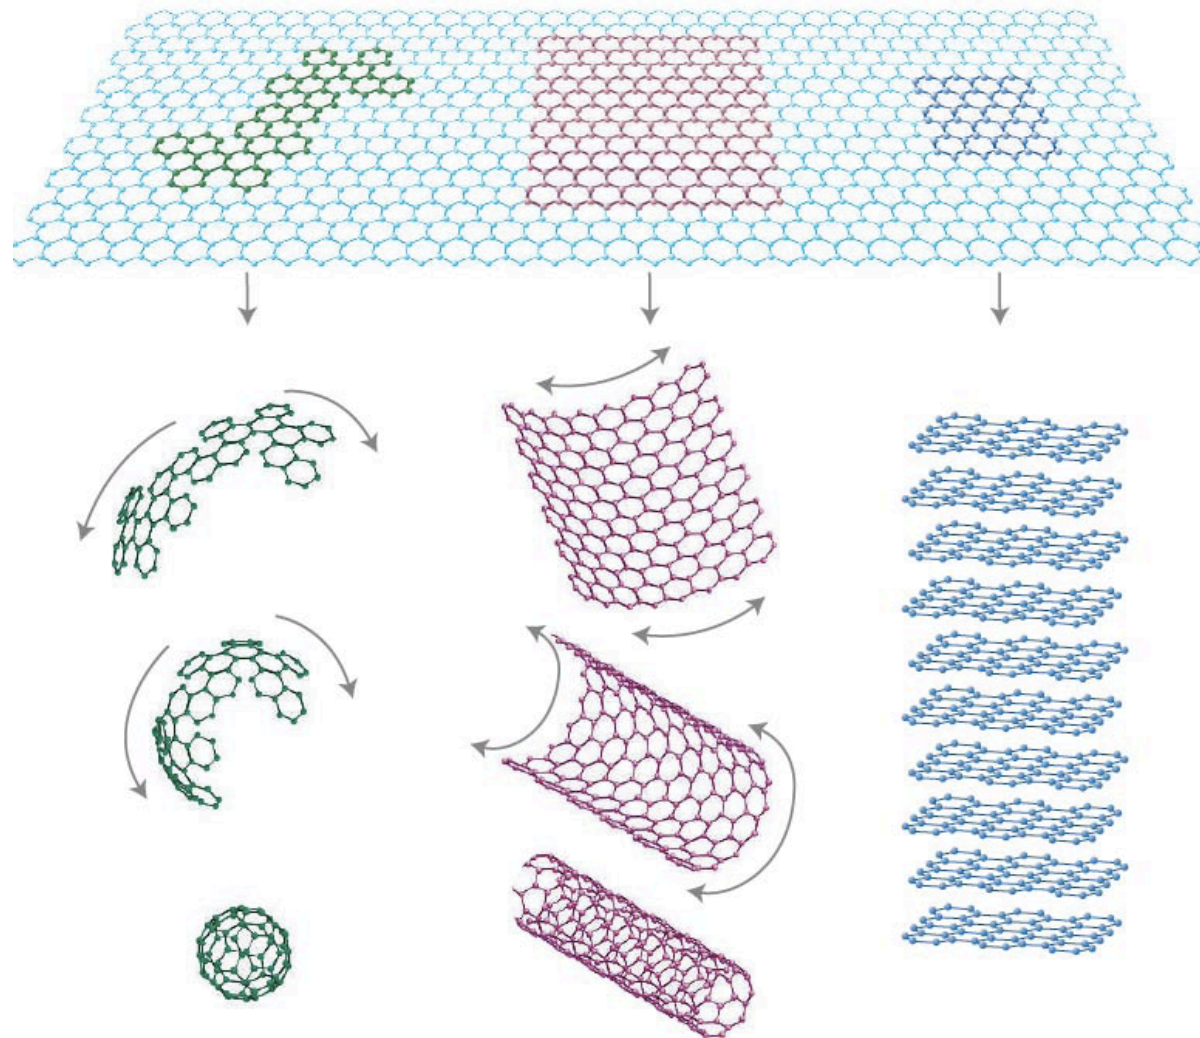

C60 fullerene molecules, carbon nanotubes, and graphite can all be thought of as being formed from graphene sheets, *i.e. single layers of carbon atoms arranged in a honeycomb lattice.*

A. K. Geim and K. S. Novoselov, *Nature Materials* 6, 183 (2007).

Detection of Nucleic Acids with Graphene Nanopores

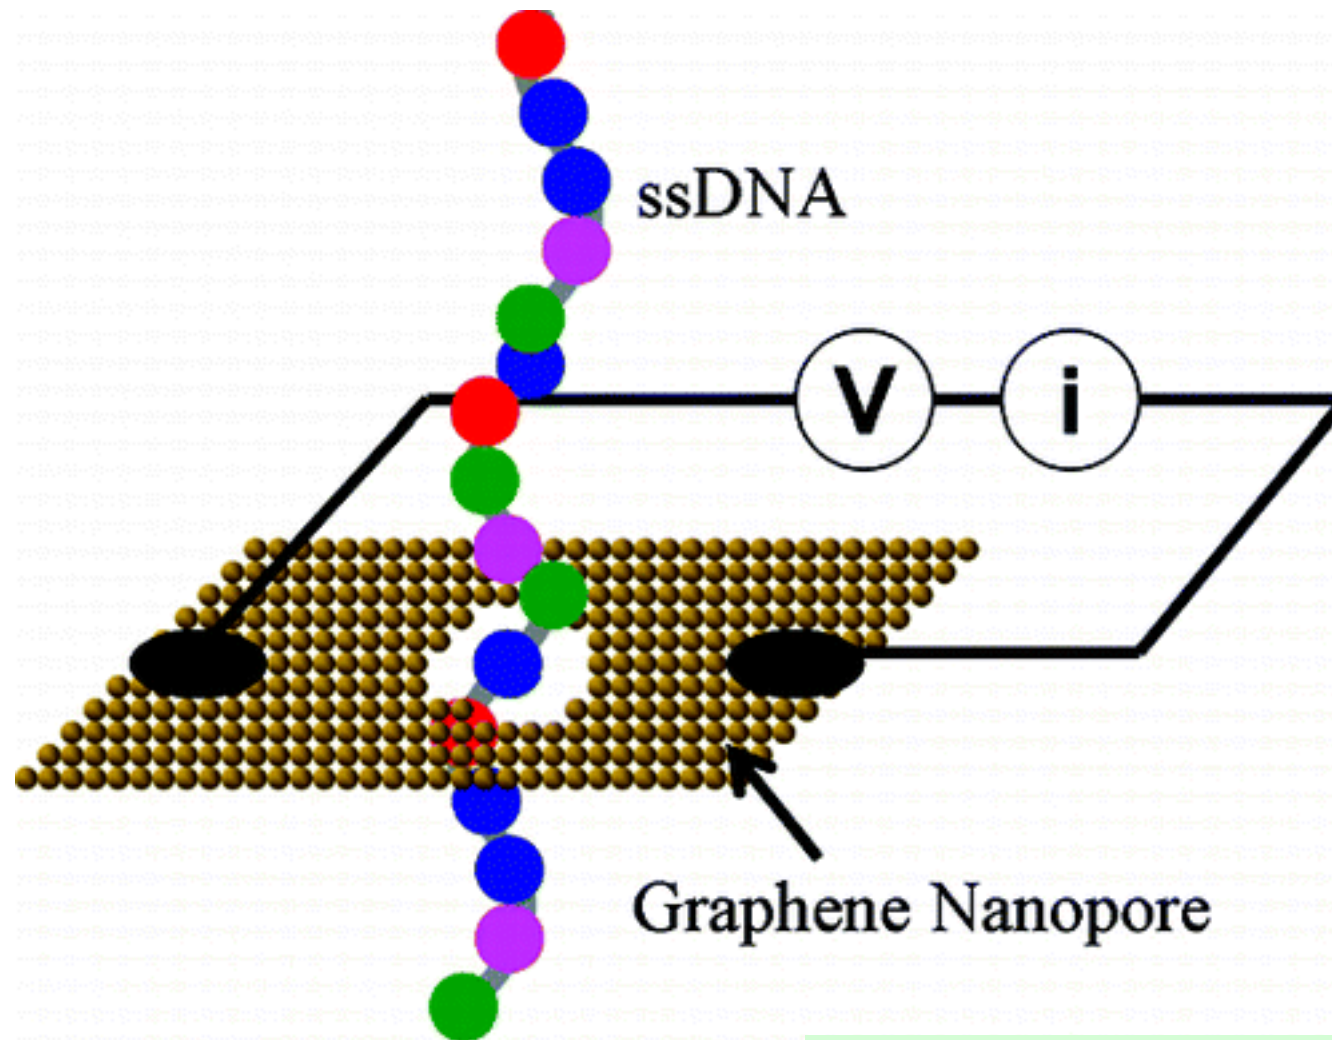


Tammie Nelson, Bo Zhang and Oleg V. Prezhdo,
Nano Lett., 2010, 10 (9), pp 3237–3242




Graphene as a subnanometre trans-electrode membrane

S Garaj *et al. Nature* 467, 190–193 (09 September 2010), doi:10.1038/nature09379

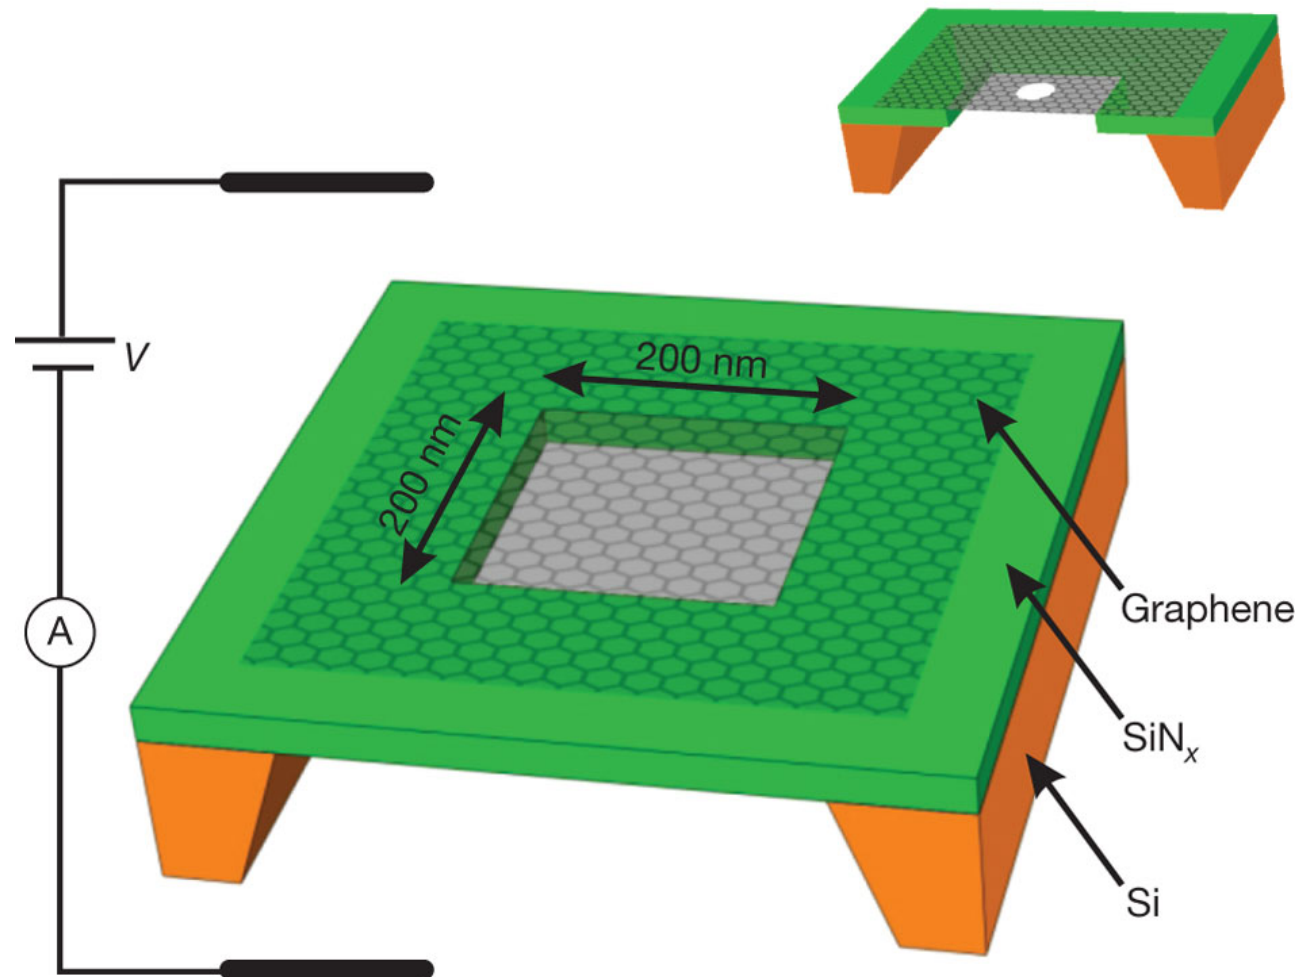

nature


Trans-electrode I – V curves

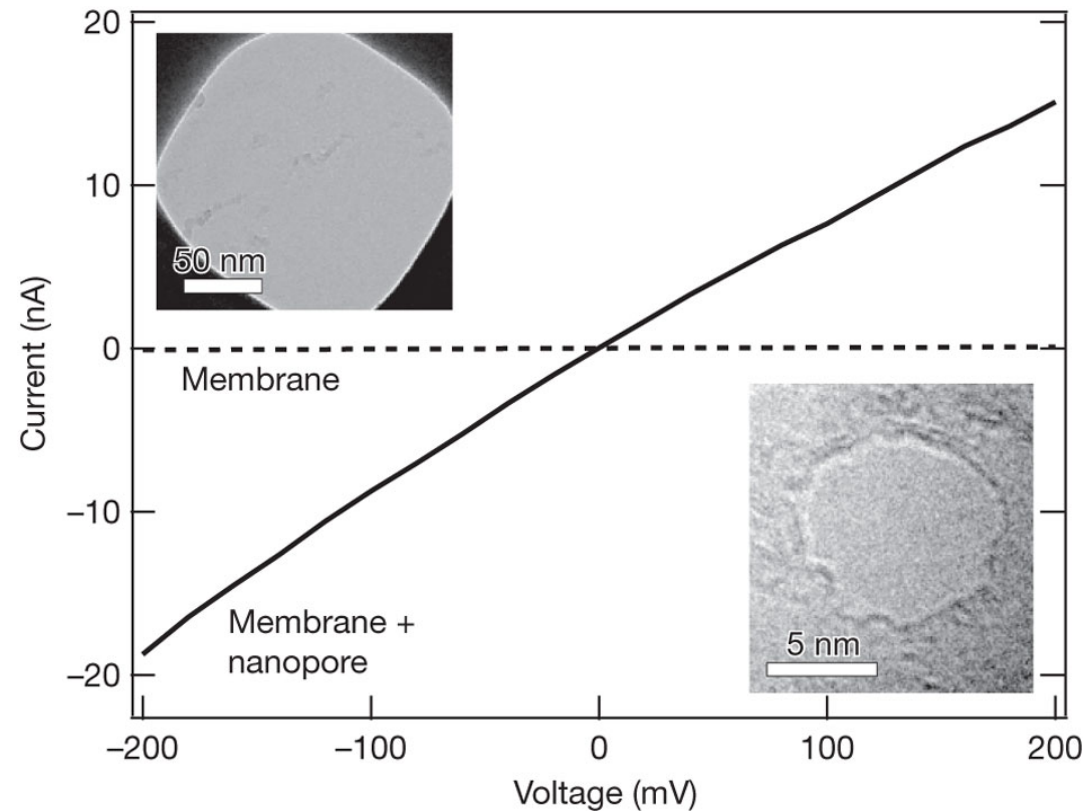

Results for an as-grown graphene membrane (dashed line) and a membrane with an 8-nm pore (solid line). The ionic conductance of the pore is quantitatively in agreement with the modelling presented in the text. Applying bias voltages in excess of ~ 250 mV gradually degraded the insulating properties of the membranes. Insets, TEM images: top, a mounted graphene membrane; bottom, the 8-nm pore.

S Garaj *et al.* *Nature* 467, 190–193 (09 September 2010)

Average nanopore current blockades versus blockade duration during DNA translocation

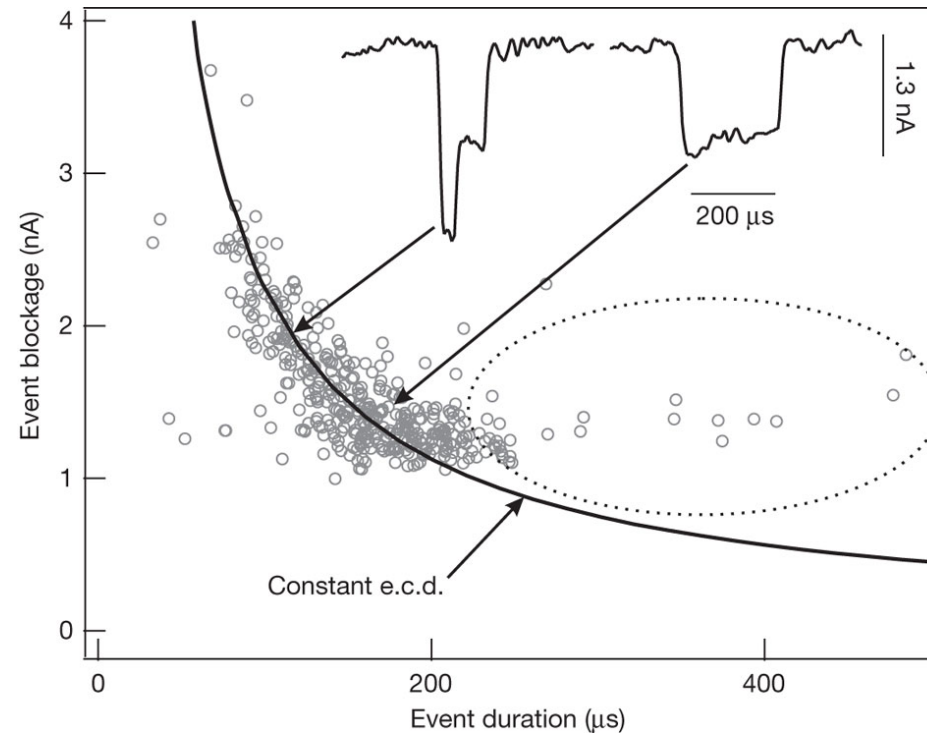

DNA ($16 \mu\text{g ml}^{-1}$) was electrophoretically driven through a 5-nm-diameter graphene pore by an applied voltage bias of 160 mV. The graphene membrane separated two fluid cells containing unbuffered 3 M KCl solutions, pH 10.4. Insets, typical current-time traces for two translocation events sampled from among those pointed to by the arrows. The hyperbolic curve corresponds to freely translocating events at a fixed e.c.d. (electronic charge deficit)

Encircled events are delayed by graphene-DNA interactions.



References:

1. Biosensors and biodetection: methods and protocols / edited by Avraham Rasooly, Keith E. Herold. New York : Humana Press, c2009.
2. Electrochemical sensors, biosensors, and their biomedical applications/ edited by Xueji Zhang, Huangxian Ju, Joseph Wang Imprint Amsterdam ; Boston :Academic Press, 2008.
3. Biosensors : a practical approach / edited by Jonathan M. Cooper, Anthony E.G. Cass Imprint New York : Oxford University Press, 2004.
4. Single-Molecule Detection in Solution Methods and Applications / edited by Christoph Zander, Jörg Enderlein, and Richard A. Keller: Wiley-VCH, 2002.